



EL769649925US



INVESTOR IN PEOPLE

The Patent Office  
Concept House  
Cardiff Road  
Newport  
South Wales  
NP10 8QQ



I, the undersigned, being an officer duly authorised in accordance with Section 74(1) and (4) of the Deregulation & Contracting Out Act 1994, to sign and issue certificates on behalf of the Comptroller-General, hereby certify that annexed hereto is a true copy of the documents as originally filed in connection with the patent application identified therein.

In accordance with the Patents (Companies Re-registration) Rules 1982, if a company named in this certificate and any accompanying documents has re-registered under the Companies Act 1980 with the same name as that with which it was registered immediately before re-registration save for the substitution as, or inclusion as, the last part of the name of the words "public limited company" or their equivalents in Welsh, references to the name of the company in this certificate and any accompanying documents shall be treated as references to the name with which it is so re-registered.

In accordance with the rules, the words "public limited company" may be replaced by p.l.c., plc, P.L.C. or PLC.

Re-registration under the Companies Act does not constitute a new legal entity but merely subjects the company to certain additional company law rules.

Signed

Dated

18 June 2001

## Patents Form 1/77

The  
Patent  
Office

1/77

Patents Act 1977  
(Rule 16)


30 AUG 2000

## Request for grant of a patent

(See the notes on the back of this form. You can also get an explanatory leaflet from the Patent Office to help you fill in this form)

The Patent Office

Cardiff Road  
Newport  
Gwent NP9 1RH

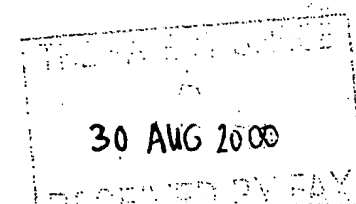

1.	Your reference	P2637A4/PAG		
2.	Patent application number (The Patent Office will fill in this part)	0021219.1		
3.	Full name, address and postcode of the or of each applicant (underline all surnames)	Hypoguard Limited Dock Lane Melton Woodbridge IP12 1PE Patents ADP number (if you know it) 4135190001 If the applicant is a corporate body, give the country/state of its incorporation United Kingdom		
4.	Title of the invention	Test Device		
5.	Name of your agent (if you have one)	DUMMETT COPP		
	"Address for service" in the United Kingdom to which all correspondence should be sent (including the postcode)	25 THE SQUARE MARTLESHAM HEATH IPSWICH IP5 3SL Patents ADP number (if you know it) 6379001		
6.	If you are declaring priority from one or more earlier patent applications, give the country and the date of filing of the or of each of these earlier applications and (if you know it) the or each application number	Country	Priority application number (if you know it)	Date of filing (day / month / year)
7.	If this application is divided or otherwise derived from an earlier UK application, give the number and the filing date of the earlier application	Number of earlier application	Date of filing (day / month / year)	
8.	Is a statement of inventorship and of right to grant of a patent required in support of this request? (Answer 'Yes' if: a) any applicant named in part 3 is not an inventor, or b) there is an inventor who is not named as an applicant, or c) any named applicant is a corporate body. See note (d))	Yes		

**Patents Form 1/77**

9. Enter the number of sheets for any of the following items you are filing with this form.  
Do not count copies of the same document

## Continuation sheets of this form

Description	17
Claim(s)	6
Abstract	1
Drawing(s)	18

10. If you are also filing any of the following, state how many against each item.

## Priority documents

## Translation of priority documents

Statement of inventorship and right to grant of a patent (Patents Form 7/77)

Request for preliminary examination and search (Patents Form 9/77) 1

Request for substantive examination (Patents Form 10/77) 1

Any other documents (please specify)

11. I/We request the grant of a patent on the basis of this application.

Signature

Date

DUMMETT COPP



30 August 2000

12. Name and daytime telephone number of person to contact in the United Kingdom  
Dr Peter A Gemmell  
01473 660600

**Warning**

After an application for a patent has been filed, the Comptroller of the Patent Office will consider whether publication or communication of the invention should be prohibited or restricted under Section 22 of the Patents Act 1977. You will be informed if it is necessary to prohibit or restrict your invention in this way. Furthermore, if you live in the United Kingdom, Section 23 of the Patents Act 1977 stops you from applying for a patent abroad without first getting written permission from the Patent Office unless an application has been filed at least 6 weeks beforehand in the United Kingdom for a patent for the same invention and either no direction prohibiting publication or communication has been given, or any such direction has been revoked.

**Notes**

- If you need help to fill in this form or you have any questions, please contact the Patent Office on 0645 500505.
- Write your answers in capital letters using black ink or you may type them.
- If there is not enough space for all the relevant details on any part of this form, please continue on a separate sheet of paper and write "see continuation sheet" in the relevant part(s). Any continuation sheet should be attached to this form.
- If you have answered 'Yes' Patents Form 7/77 will need to be filed.
- Once you have filled in the form you must remember to sign and date it.
- For details of the fee and ways to pay please contact the Patent Office.

- 1 -

## TEST DEVICE

## BACKGROUND OF THE INVENTION

## 5 1. Field of the Invention

The present invention relates to a test device for measuring the concentration of an analyte in a fluid sample, notably to a test device for analysing blood  
10 glucose or other analytes in bodily fluids.

## 2. Description of the Prior Art

Diabetics regularly need to test samples of their blood to  
15 determine the level of blood glucose. The results of such tests may be used to determine levels of medication needed to treat the diabetes at the time. In one known type of system, disposable sensors are used to test the blood. The sensors typically take the form of test strips which  
20 are provided with a reagent material that will react with blood glucose to produce an electrical signal. Conductive tracks on the test strip relay the electrical signal to a meter which displays the result. After a sample of blood has been applied to the test strip and the measurement has  
25 been taken, the test strip is disposed of. In order to couple the conductive tracks on a test strip with the meter, the test strip needs to be inserted into a sensor holder prior to the start of testing. The sensor holder has corresponding electrodes which are brought into  
30 electrical contact with the conductive tracks of the test strip. Test devices are known in which a plurality of test strip are provided on a cartridge disc. Each strip is housed in its own sensor slot, and means are provided to eject a test strip from its slot when required, and to  
35 automatically locate it in a sensor holder. Examples of

- 2 -

test devices with test strip dispensers are described in US Patent No. 5,660,791, European Patent Application No. 0 732 590, and European Patent Application No. 0 738 666.

5 A problem with test strips is that they have only a limited shelf life, and exposure of test strips to the atmosphere reduces the shelf life further. Test strips open to the atmosphere will typically have a shelf life of about two to three months, whereas test strips which are  
10 sealed from the atmosphere will have a shelf life of about six to 12 months.

It has been proposed in WO 94/10558 to provide a stack of disposable test elements in a cylindrical housing, the  
15 stack being urged towards a test station to form a liquid-proof seal. In DE 196 39 226 A1 it is proposed to provide a test device with a cartridge that may have a plurality of chambers containing test strips, each of which chambers may be individually sealed to preserve the shelf life of  
20 the strips therein. A user removes the seal for each chamber when required, and a timing circuit may be activated either by the user or when the cartridge is pushed into the device. After a set time period has elapsed, an alarm or other indication reminds the user  
25 that the time period for using the strips has elapsed.

It is an object of the present invention to provide an improved test device.

### 30 SUMMARY OF THE INVENTION

According to an aspect of the present invention there is provided a test device for testing of analyte concentration in a fluid to be applied thereto, the device  
35 comprising:

- 3 -

- a) a plurality of sensors arranged in a stack, each of said sensors carrying reagent means for producing an electrical signal in response to the concentration of analyte in an applied fluid, each of said sensors having a plurality of electrode tracks for transmitting said electrical signal;
- b) a housing having an opening therein and containing the said stack of sensors;
- c) electrical contacts mounted in relation to the housing for engaging with electrode tracks on a sensor at an engagement location;
- c) a meter connected to the said electrical contacts, having electronics means for producing a signal output which is dependent on the electrical signal from a sensor when the sensor is engaged with the said contacts;
- d) a transport member rotatably mounted in the opening of the housing, having an axis of rotation which spans the opening and having an outer surface which is provided with a recessed region adapted to receive a single sensor from the stack;
- e) spring means within the housing which urge the stack of sensors towards the transport member and which urge a single sensor into the said recess when the recess is suitably aligned adjacent to the stack;
- f) sealing means for making a moisture tight seal between the transport member and the stack when the transport member is in a specified rotational position; and
- g) wherein rotation of the transport member with a sensor in the recessed region will transport the sensor to the engagement location or to a position where the sensor can be pushed to the engagement location, whereby electrode tracks of the sensor can engage with the said electrical contacts.

35

- 4 -

With the transport member in a start or home position, the sealing means keeps moisture from sensors in the stack when the device is not being used. The device may be factory assembled under controlled temperature and humidity conditions, and kept sealed until a user is ready to use a sensor. In a preferred embodiment the sealing means also provide a moisture-proof seal when the sensor is in the engagement location, so that sensors in the stack are protected while an analyte measurement is being taken.

The invention will be described with reference to the testing of glucose concentrations in blood, but it will be understood that the invention is not limited to this embodiment and is of general applicability for testing analytes in bodily and other fluids.

The transport member may take the sensor to the engagement location by rotational motion alone. Additional pushing means may be provided to translate the test strip to the engagement location. Such pushing means may be provided by a captured pusher which engages with a track on the housing so as to move the test strip during rotation of the transport member. Alternatively, separately actuatable pushing means could be provided to push the sensor to the engagement location after rotation of the transport member to a suitable position.

The electrical contacts may be brought automatically into contact with electrode tracks on the sensor in the engagement location, for example by means of spring biasing. Alternatively, the user could move the electrical contacts to achieve the necessary contact at the engagement location.

35

- 5 -

After a measurement has been taken, it would be possible to remove the used sensor from the engagement location by manual intervention from the user. However, to avoid the need for handling of the used sensor it is preferred that  
5 the transport member can be further rotated from the engagement location to an exit location at which the sensor can fall out or be pushed out by ejection means.

After completion of a test measurement, and ejection of  
10 the used sensor, the transport member is returned or advanced to the start position. This may be done manually by the user or by means of a motor. The transport member is preferably urged by a return spring to return to the start position.

15 For simplicity the transport member is preferably circular in cross section, for example a cylindrical feed barrel. However the transport member could have a sectional shape that is not circular, for example oval, square or  
20 triangular.

The sealing means may be provided on an external surface of the transport member, or separate sealing means may be provided that make a seal between the transport member and  
25 the housing or the stack of sensors. Where the seal is made with the housing, the opening in which the transport member is mounted must of course be the only opening to the inside of the housing. In a preferred embodiment the sealing means comprises a retractable shroud which  
30 surrounds the stack of sensors and which sealingly engages with the transport member when in an extended configuration. In another preferred embodiment, the sealing means is provided by a seal on a door which opens and closes the opening according to the rotational  
35 position of the transport member. The door may be



- 6 -

provided with one or more teeth to restrain movement of the stack, and the transport member may be provided with one or more blades to take over the restraining function from the teeth when the door is open, prior to the  
5 recessed region of the transport member being brought into register with the stack. This embodiment has the advantage that the door may remain closed, and the seal intact, at all times except for the brief period when a sensor is being loaded and taken to the engagement  
10 location. The sealing means may be formed from any suitable material, for example natural or synthetic rubber.

The sensors may be conventional test strips of known  
15 construction. The invention will for convenience be described hereinafter with reference to test strips; however it is to be understood that other shapes of sensor could also be employed.

20 The invention provides a test device in which test strips are dispensed via a rotationally mounted transport member so that each test strip is conveniently brought to a location where it can engage with meter contacts and where it can receive a drop of fluid. Accordingly, another  
25 aspect of the invention provides a test device for testing of analyte concentration in a fluid to be applied thereto, comprising: a housing containing a stack of test strips and having an opening therein; a transport member rotatably mounted in the opening of the housing, having an  
30 axis of rotation which spans the opening; the transport member having a recessed region adapted to receive a single test strip; and spring means which urge the stack towards the transport member; wherein rotation of the transport member with a test strip in the recessed region  
35 thereof will bring the said test strip to an engagement

- 7 -

location at which it can be engaged with electrical contacts of a meter and at which the test strip will be accessible to permit a user to apply a drop of fluid thereto.

5

In a preferred embodiment, each test strip comprises a base member having a working area to which the fluid is to be applied, containing the reagent means, and a non-working area adjacent to the working area, wherein the  
10 total thickness of the test member in at least a portion of the non-working area is at least as great as the total thickness of the test member in the working area.

15

By making the non-working area at least as thick as the working area, scuffing or abrasion of the working area in a stack can be reduced. Moreover, if a compressive load is applied to a stack of the test members, this may be spread out over a greater area, thereby reducing the possibility of compressive damage to the working area.

20

In a preferred embodiment, at least a part of the non-working area is of greater total thickness than the thickness of the working area. This further reduces the likelihood of damage to the working area by scuffing or  
25 abrasion when in a stack. The difference in thickness is preferably from 1 to 20  $\mu\text{m}$ , notably from 5 to 10  $\mu\text{m}$ .

30

To build up the working area, a plurality of layers are sequentially applied to the base layer, for example by  
screen printing, typically with curing or drying steps between the application steps. The layers which are printed typically comprise electrode patterns, a reagent layer, and a mesh layer (for spreading out an applied fluid). As a result of the application of these layers,  
35 the working area of a conventional electrochemical test

- 8 -

strip is typically about 100  $\mu\text{m}$  thicker than the non-working area, which contains the electrode tracks and, typically, a dielectric layer. A stack of 100 test strips will therefore be about 10 mm thicker in the working area than in the non-working area. In a test strip in accordance with the present invention, at least a part of the non-working area may be made thicker by any suitable means. Suitable means include, for example: a printed relief ink; an applied pad or tape; embossing of the base layer or an intermediate layer; or an extension of the mesh layer from the working area.

Further objects and advantages of the invention will be apparent as the description proceeds.

15

- 9 -

## DETAILED DESCRIPTION OF THE DRAWINGS

The invention will now be further described, by way of example, with reference to the following drawings in which:

- Figure 1 shows perspective views of a test device in accordance with a first embodiment of the present invention;
- Figure 2 shows horizontal sectional views through the device of Figure 1a, along the line C-C of Figure 4) with the sealing means extended and retracted;
- Figures 3 and 4 show vertical sectional views along the lines A-A and B-B respectively of Figure 2;
- Figures 5 and 6 show vertical sectional views corresponding to those of Figures 3 and 4 respectively, but with the transport member progressively rotated;
- Figure 7 shows respective sectional views along the lines E-E, F-F and G-G of Figures 5 and 6;
- Figure 8 shows perspective views of a test device in accordance with a second embodiment of the present invention;
- Figure 9 is a top plan view of the test device of Figure 8a;
- Figure 10 is a sectional view along the line A-A of Figure 9;

- 10 -

Figure 11 is a sectional view along the line B-B of Figure 10;

5 Figure 12 shows sectional views corresponding to that of Figure 10, with the transport member at different rotational positions;

10 Figure 13 shows top plan views similar to Figure 9, with a test strip in different positions during the course of a test measurement;

15 Figure 14 shows perspective views of a test device in accordance with a third embodiment of the present invention;

Figure 15 is a top plan view of the test device of Figure 14a;

20 Figure 16 is a sectional view along the line A-A of Figure 15;

Figure 17 is a sectional view along the line B-B of Figure 16;

25 Figure 18 shows sectional views corresponding to that of Figure 16, with the transport member at different rotational positions;

30 Figure 19 shows top plan views similar to Figure 15, with a test strip in different positions during the course of a test measurement; and

35 Figure 20 is a top plan view of a test strip in a preferred embodiment of the invention.

- 11 -

## DETAILED DESCRIPTION

In the embodiment illustrated in Figures 1 to 7, a test device for measuring glucose concentration in blood comprises a housing 2 which houses a stack of test strips 16 in a magazine housing 18. A transport member 4 (in this example, a feed barrel which is circular in cross section) is rotatably mounted in an opening of the housing 2 and has an axis of rotation which spans the opening. As will be described below, the feed barrel 4 has a recessed portion 12 which receives and transports a single test strip 16 from the stack in the magazine from a start position (Figure 1a) to an engagement location (Figure 1b) where electrode tracks 50 on the test strip engage with electrical contacts mounted in the housing and connected to a meter. With the test strip 16 in the engagement location a user can apply a drop of blood to the working area 42 of the test strip 16. The housing has mounted thereon a meter comprising a PCB 6 and display means 8 (in this example, an LCD) for displaying a readout of blood glucose concentration. Glucose concentration values from previous samples can be retained and displayed by operation of a memory button 10 on the PCB. Further rotation of the feed barrel 4 brings the used test strip 16 to an opening 14 in the housing 4 through which the test strip can be ejected or removed.

As shown in Figures 2 to 6, test strips 16 in the magazine housing 18 are protected by a moisture-proof retractable sealing member 20, which is tightly fitted around ribs 21 on the magazine housing 18. The free end of the retractable sealing member 20 is located in a groove 26 which surrounds the recess 12 where the test strip 16 is located in the start position. The retractable sealing member 20 is engaged by a movable support collar 22. In

- 12 -

the start position, a constant tension magazine spring 24 urges the stack of test strips against the feed barrel 4 so that a single test strip 16 lies flat in the recess 12. Only a single spring is necessary, although an optional  
5 second spring is also illustrated.

When the user initiates turning of the feed barrel 4 in the start position (Figures 2a, 3a, 4a), the first thing that happens is that the support collar 22 is moved away  
10 from the feed barrel 4 so as to disengage the free end of the retractable sealing member 20 from the groove 26, thereby permitting rotation of the feed barrel 4 (Figures 2b, 3b, 4b).

15 With the retractable sealing member 20 in a retracted configuration, the feed barrel 4, carrying a single test strip 16, is turned by the user (Figures 5a, 6a) until the test strip 16 is at the top of the feed barrel 4, as shown in Figures 5b and 6b. At the same time, a captured pusher  
20 28, behind the test strip 16, engages a helical track 30 (Figures 7a, 7b) in the housing 2. This track 30 moves the pusher 28 forward which in turn moves the test strip 16 out of the housing 2 and into the engagement location. As the test strip 16 reaches the engagement location, it  
25 flexes a contact (not shown) into a "wake up" position which activates the meter into a ready for use state. The feed barrel 4 is turned against a return spring (not shown). In the engagement location, the barrel 4 is held by a "ball point pen" type mechanism (not shown). After a  
30 reading has been taken, further turning of the feed barrel 4 (Figures 5c, 6c, 7c) brings the recess 12 and used test strip 16 to the opening 14 where the test strip 16 may drop out or urged out by ejection means. On release of the feed barrel 4 from the exit location, the return

- 13 -

spring returns the feed barrel 4 to the start position, where the next test member 16 from the stack engages in the recess 12. The process can then be repeated until all test members have been used up. The device may then be  
5 discarded.

In the embodiments shown in Figures 8 to 19, parts with similar structure and function to the first embodiment are given the same reference number.

10

In the second embodiment shown in Figures 8 to 13, the feed barrel 4 is partially cutaway so that a test strip 16 is only partially supported in the recess 14. The part of the housing 2 in which the feed barrel 4 is mounted is  
15 also cutaway, so that a used test strip which is turned so that it exits the housing can drop out or be ejected. A seal 34 is provided on part of the full length outer surface of the feed barrel 4 so that, in the start position illustrated in Figures 8a and 9 to 11, the seal  
20 34 creates a moisture tight seal between the test strips 16 and the feed barrel 4.

From the start position, a user brings a test strip 16 to the engagement location where it engages with electrical  
25 contacts 32 on the housing 2 by the steps illustrated in Figures 12a to 12d, 13a and 13b. The feed barrel 4 is provided with a drive axle 36. The user turns the drive axle 36 in the direction of the arrow as shown in Figure 12a, against the force of a return spring 38, to the feed  
30 position shown in Figure 12b. Here the recess 12 is brought into register with the test strips 16, and a single test strip 16 locates in the recess 12. The user then releases the drive axle 36, and the return spring 38 carries the feed barrel 4 back to the start position via  
35 the intermediate position shown in Figures 12c and 13a.



- 14 -

With the electrode tracks on the test strip 16 engaged with the electrical contacts 32 of the meter, the user now takes a reading of blood glucose concentration. The seal 34 once again seals off the test strip cartridge from atmospheric moisture, so that test strips in the cartridge are protected from moisture while the reading is being taken.

After the reading has been taken, the user turns the drive axle 36 in the direction of the arrow 35 (Figure 12e) and the used test strip 16 is either permitted to drop from the recess 12 or is positively ejected (Figures 12e, 13). The user then releases the drive axle 36 and the feed barrel is returned to the start position by the return spring 38. The cartridge of test strips is kept sealed from moisture at all times except for short periods when a test strip is being loaded and when the used test strip is being ejected.

Turning now to Figures 14 to 19, the third embodiment illustrated is similar to the second embodiment, but includes special means for retaining sensors in the magazine and for sealing the magazine even during ejection of a used test strip.

The feed barrel 4 is provided with a separate magazine door 52 which has a door seal 66. When the door 52 is closed, the door seal 66 protects test strips 16 from atmospheric moisture. A plurality of fingers 54 are provided on the door, and these fingers keep the test strips 16 away from the door seal 66. The door 52 is pivotally mounted to a pivot point 56, and is provided with arms 58. Pulling or pushing on an arm 58 causes pivoting of the door 52. Within the feed barrel 4 there is provided an actuating member 60 which includes a pair

- 15 -

of spaced apart arms 68 and a pair of spaced apart fingers 64. The end of each finger 64 is journaled between a pair of arms 58 on the magazine door 52. At the end of each arm 68 of the actuating member there is provided a blade 62. To take a blood glucose reading, the following actions are performed. From the start position shown in Figure 16, the user turns the feed barrel 4 in the direction of the arrow shown in Figure 18a. The actuation member 60 also turns, and the fingers 64 pull on an arm 58 of the magazine door 52. The door 52 pivots and begins to withdraw from the magazine. The stack of test strips 16 follows, urged by the spring 24 and restrained by the teeth 54. At the same time, the blades 62 are rotated so that they lie between the teeth 54 and take over the job of restraining the test strips 16 (Figure 18a). As the feed barrel 4 is further rotated (Figure 18b) the blades 62 move out of line with the magazine opening and the recess 12 on the feed barrel moves into alignment with the test strips 16. A single test strip 16 lies flat in the recess 12. The user then permits the return spring 38 to turn the feed barrel 4 in the direction of the arrow shown in Figure 18c, so as to bring the test strip 16 in the recess 12 to the engagement location (Figure 18d). As the barrel 4 turns, initially the blades 62 and subsequently the teeth 54 push the stack of test strips 16 further back into the magazine. The magazine door 52 is closed again and the door seal 66 again seals the inside of the magazine from moisture. After a test reading has been taken, the user turns the feed barrel in the direction shown by the arrow in Figure 18e, and the used test strip is discarded. During testing and during discarding of the test strip, the door 52 remains closed by virtue of lost motion between the fingers 64 on the actuating member 60 and the arms 58 of the door 52. On release of the drive axle 36, the return spring 38 restores the device to the

- 16 -

start position and the process can begin again.

The test strip 16 shown in Figure 20 comprises a planar base member 38, in this example of poly(butylene terephthalate) (PBT) (Valox® FR-1 from GE Plastics). The strip is 30 mm x 5.5 mm, and 0.5 mm thick. A working area 40 is of conventional construction, comprising a plurality of electrodes, a reagent layer in intimate contact with the electrodes, and a mesh layer for spreading out a drop of fluid to be received on the working area. Electrode tracks 48, for example of carbon, in the non-working area 44 of the test strip are connected to the electrodes in the working area 40 in known manner. Also in known manner, a dielectric layer 42 is printed around the working area 40 so as to overlie a portion of the electrode tracks 48, leaving just the ends of the tracks exposed for connection to corresponding electrodes 32 on the meter. The layers are applied to the base member as inks, by screen printing. Each ink layer is about 10 to 20  $\mu\text{m}$  thick, and the mesh is about 59 to 67  $\mu\text{m}$  thick. The working area 40 has a total thickness which is about 100  $\mu\text{m}$  thicker than the non-working area 44 up to the dielectric layer 42.

To increase the thickness of parts of the non-working area, a high relief ink 46 has been printed in four strips. The high relief ink has a dried thickness such that the total thickness of the non-working area to which the high relief ink 46 has been applied is slightly greater than the total thickness of the test strip in the working area 40. Thus, when a stack of such test strips 16 is formed, and a compressive load is applied to the stack by the spring 24, the working area 40 will not bear all the compressive load. Scuffing of the test area will

- 17 -

be reduced compared to a conventional test strip in which the working area stands proud of the non-working area.

5 Although this embodiment has been illustrated with reference to the use of a high relief ink printed in strips, it will be understood that it is not limited to this embodiment. The ink could be printed as a continuous block, and it could entirely surround the working area if desired. Instead of, or in addition to, the high relief  
10 ink, other means could also be provided to increase the thickness of the non-working area, for example: an applied pad or tape; embossing of the base layer or an intermediate layer; or an extension of the mesh layer from the working area into the non-working area.

15 It is appreciated that certain features of the invention, which are for clarity described in the context of separate embodiments, may also be provided in combination in a single embodiment. Conversely, various features of the  
20 invention which are, for the sake of brevity, described in the context of a single embodiment, may also be provided separately or in any suitable subcombination.

25 Although the invention has been described with reference to a test device for measuring blood glucose concentration, it is to be understood that the invention is not limited to this application. The invention may be used in the determination of any analyte in a fluid by the use of suitable reagents in the test strip. Such reagents  
30 are well known to those skilled in the art.

- 18 -

## CLAIMS

1. A test device for testing of analyte concentration in a fluid to be applied thereto, the device comprising:
- 5 a) a plurality of sensors arranged in a stack, each of said sensors carrying reagent means for producing an electrical signal in response to the concentration of analyte in an applied fluid, each of said sensors having a plurality of electrode tracks for transmitting said
- 10 electrical signal;
- b) a housing having an opening therein and containing the said stack of sensors;
- c) electrical contacts mounted in relation to the housing for engaging with electrode tracks on a sensor at
- 15 an engagement location;
- c) a meter connected to the said electrical contacts, having electronics means for producing a signal output which is dependent on the electrical signal from a sensor when the sensor is engaged with the said contacts;
- 20 d) a transport member rotatably mounted in the opening of the housing, having an axis of rotation which spans the opening and having an outer surface which is provided with a recessed region adapted to receive a single sensor from the stack;
- 25 e) spring means within the housing which urge the stack of sensors towards the transport member and which urge a single sensor into the said recess when the recess is suitably aligned adjacent to the stack;
- f) sealing means for making a moisture tight seal
- 30 between the transport member and the stack when the transport member is in a specified rotational position; and
- g) wherein rotation of the transport member with a sensor in the recessed region will transport the sensor to
- 35 the engagement location or to a position where the sensor

- 19 -

can be pushed to the engagement location, whereby electrode tracks of the sensor can engage with the said electrical contacts.

5 2. A test device as claimed in claim 1, wherein the sensors are stacked in a magazine within the housing, the magazine having a single opening which faces the transport member.

10 3. A test device as claimed in claim 2, wherein a first end of the sealing means forms a seal around the magazine and a second end of the sealing means locates in a groove in the transport member to form a seal therewith when the recessed region of the transport member is in register  
15 with the stack of sensors.

4. A test device as claimed in claim 3, wherein the sealing means comprises a retractable sleeve which sealingly engages in the groove of the transport member  
20 when in an extended configuration and which does not form a seal with the transport member when in a retracted configuration.

5. A test device as claimed in any one of the preceding  
25 claims, wherein a pusher is provided to impart translational motion to a sensor mounted in the said recessed region during and/or after rotation of the transport member so as to bring the sensor to the engagement location.

30 6. A test device as claimed in claim 5, wherein the pusher is mounted on the transport member and a portion of the pusher is located in a helical track in the housing whereby rotation of the transport member imparts  
35 translational motion to the pusher.

- 20 -

7. A test device as claimed in claim 1, wherein the said opening is the only opening to the inside of the housing, and wherein the sealing means comprises a seal which is  
5 secured in relation to an outer surface of the transport member and which seals the opening of the housing when the transport member is in a specified rotational position.

8. A test device as claimed in claim 2, wherein the  
10 sealing means comprises a seal which is secured in relation to an outer surface of the transport member and which seals the opening of the magazine when the transport member is in a specified rotational position.

9. A test device as claimed in claim 1, wherein the said opening is the only opening to the inside of the housing, and wherein the sealing means comprises a seal provided on  
15 a door which is adapted to fit the said opening so that the moisture tight seal is effected by closure of the door; wherein the door is operatively connected to the  
20 transport member so that the door will be open when the transport member is in a first rotational position and closed when the transport member is in a second rotational position.

25 10. A test device as claimed in claim 2, wherein the sealing means comprises a seal provided on a door which is adapted to fit the opening of the magazine so that the moisture tight seal is effected by closure of the door;  
30 wherein the door is operatively connected to the transport member so that the door will be open when the transport member is in a first rotational position and closed when the transport member is in a second rotational position.

35 11. A test device as claimed in claim 9 or claim 10,

- 21 -

wherein the door is provided with one or more teeth which restrain movement of the stack of sensors against the force of the spring means.

5 12. A test device as claimed in claim 11, wherein the transport member is provided with at least one blade which takes over the function of restraining the stack of sensors when the door is opened.

10 13. A test device as claimed in any one of claims 9 to 12, wherein the door is pivotally mounted in relation to the housing.

15 14. A test device as claimed in any one of the preceding claims, wherein the transport member is operationally connected to a return spring which urges the transport member to adopt a specified rotational position at which the sealing means can provide a moisture proof seal between the stack of sensors and the transport member.

20 15. A test device as claimed in any one of the preceding claims, wherein a portion of the sensor to which a fluid sample is to be applied is not supported by the transport member when in the engagement location.

25 16. A test device as claimed in any one of the preceding claims, wherein the transport member has an external profile which is substantially circular in cross section.

30 17. A test device for testing of analyte concentration in a fluid to be applied thereto, comprising: a housing containing a stack of test strips and having an opening therein; a transport member rotatably mounted in the opening of the housing, having an axis of rotation which  
35 spans the opening; the transport member having a recessed



- 22 -

- region adapted to receive a single test strip; and spring means which urge the stack towards the transport member; wherein rotation of the transport member with a test strip in the recessed region thereof will bring the said test strip to an engagement location at which it can be engaged with electrical contacts of a meter and at which the test strip will be accessible to permit a user to apply a drop of fluid thereto.
- 10 18. A test device as claimed in claim 17, further including sealing means which make a moisture-proof seal between the transport member and the stack when the transport member is in a specified rotational position.
- 15 19. A test device as claimed in any one of the preceding claims, wherein each sensor in the or each stack comprises a base member having a working area to which the fluid is to be applied, containing the reagent means, and a non-working area adjacent to the working area, wherein the total thickness of the sensor in at least a portion of the non-working area is at least as great as the total thickness of the sensor in the working area.
- 20 20. A test device as claimed in claim 19, wherein the total thickness of the sensor in at least a part of the non-working area is greater than the total thickness of the sensor in the working area.
- 25 21. A test device as claimed in any one of the preceding claims, suitable for use in testing glucose concentration in blood.
- 30 22. A test device for testing of analyte concentration in a fluid to be applied thereto, substantially as herein described with reference to or as shown in Figures 1 to 7
- 35

30-08-00 16:40 01473 660612  
30-AUG-2000 16:48 FROM DUMMETT COPP

P.28 R-249 Job-646  
TO PATENT OFFICE P.28/47

- 23 -

or 8 to 13 or 14 to 19 of the drawings.

- 24 -

## ABSTRACT

### TEST DEVICE

5 A test device for testing of analyte concentration in a  
fluid comprises: a housing (2) having an opening and  
containing a stack of sensors (16); a transport member (4)  
rotatably mounted in the opening of the housing, having an  
axis of rotation which spans the opening; a spring (24)  
10 which urges the stack against the transport member; and  
sealing means (20, 34) for making a moisture tight seal  
between the transport member and the sensors when the  
transport member is in a specified rotational position.  
An outer surface of the transport member has a recessed  
15 region (12) which is adapted to receive a single sensor  
from the stack. Rotation of the transport member with a  
sensor in the recessed region transports the sensor to a  
location where it can be connected to a meter (6, 8) and  
receive a drop of fluid to be tested.

20

Figure 3a

1/18

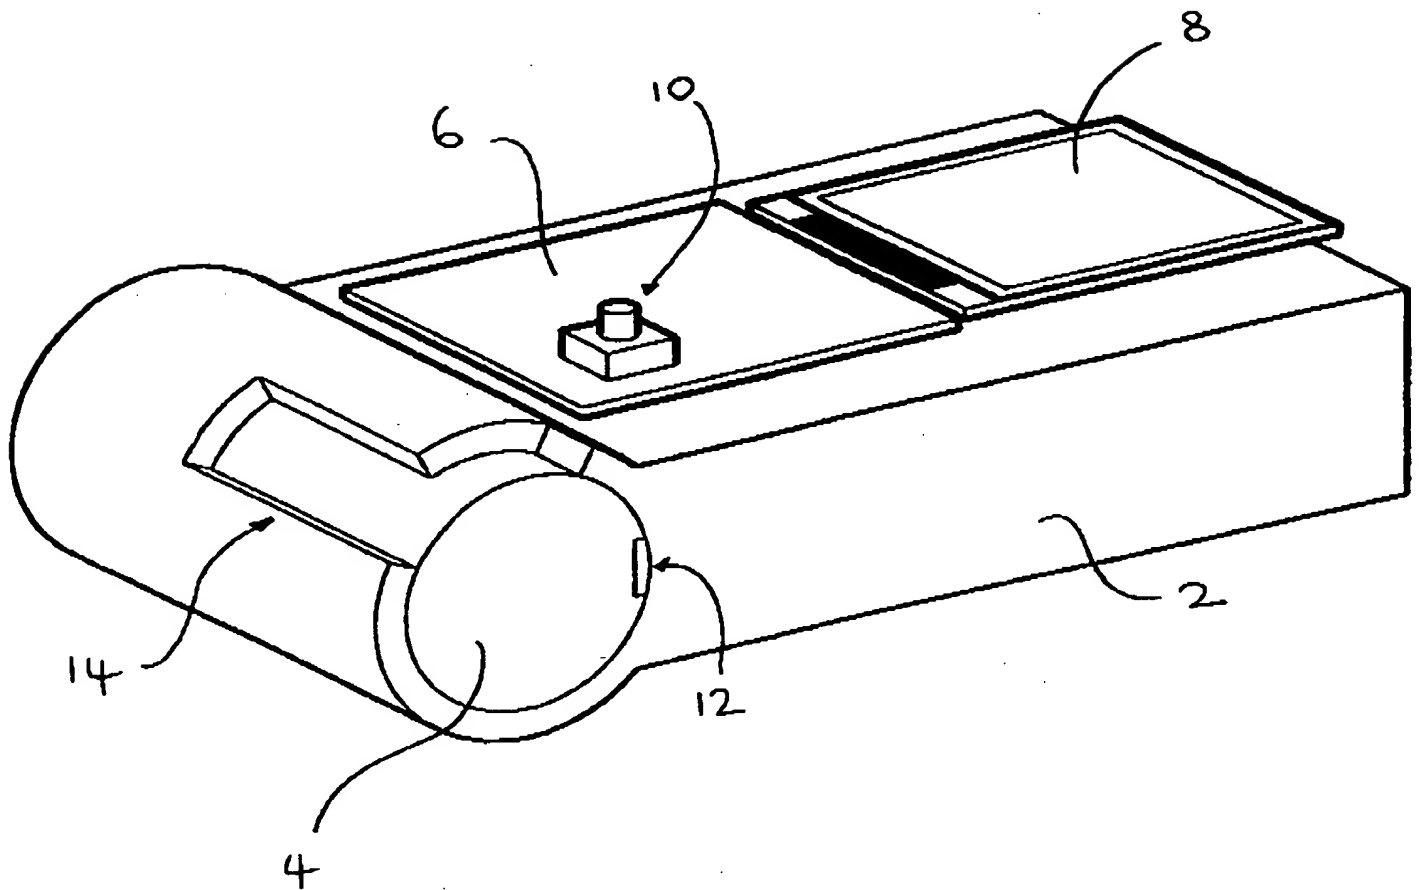


FIG. 1a

2/18







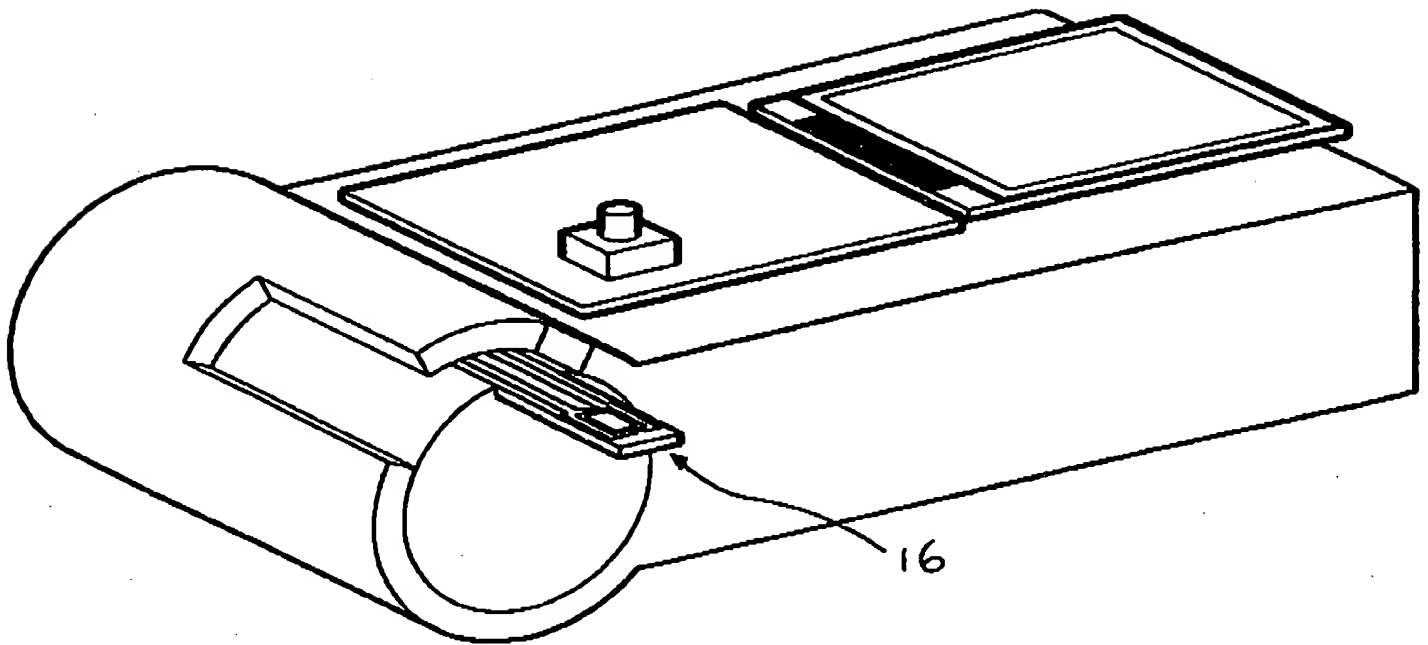





FIG. 1b

3/18

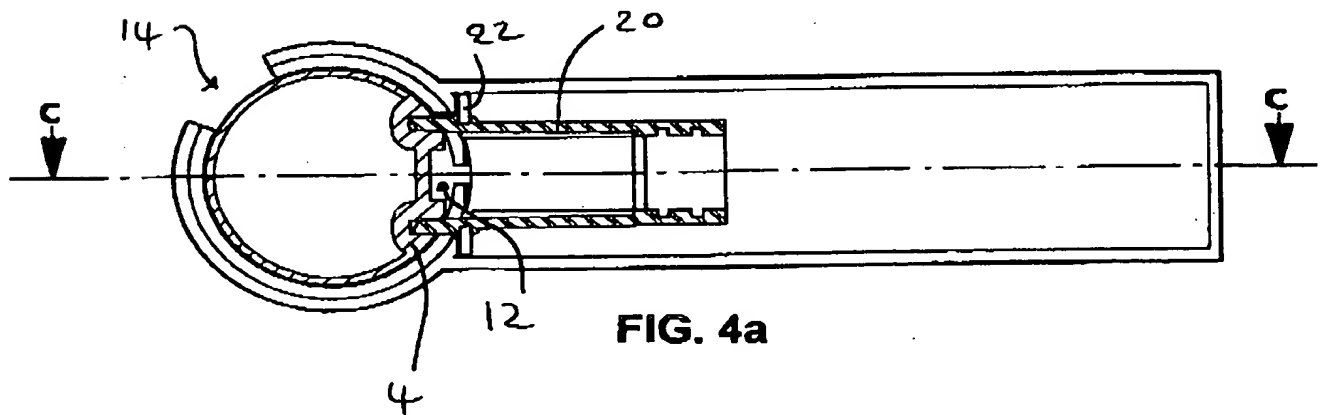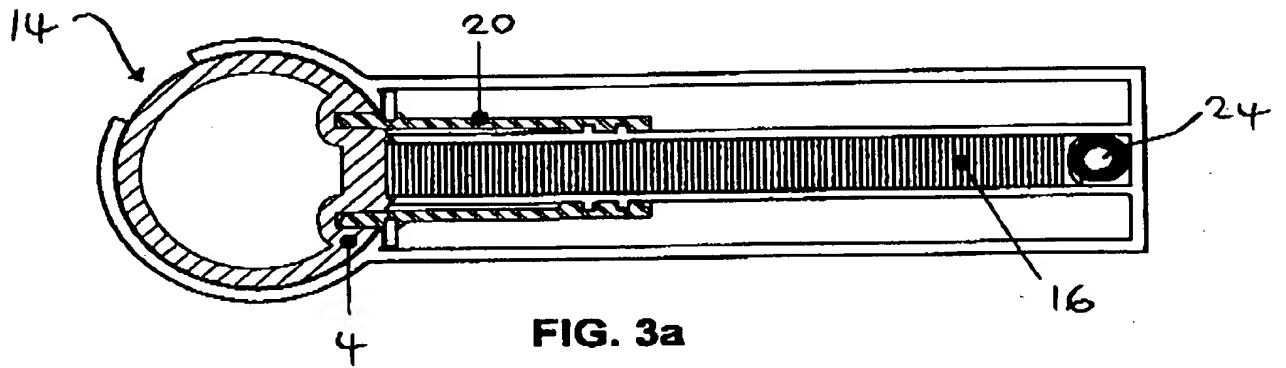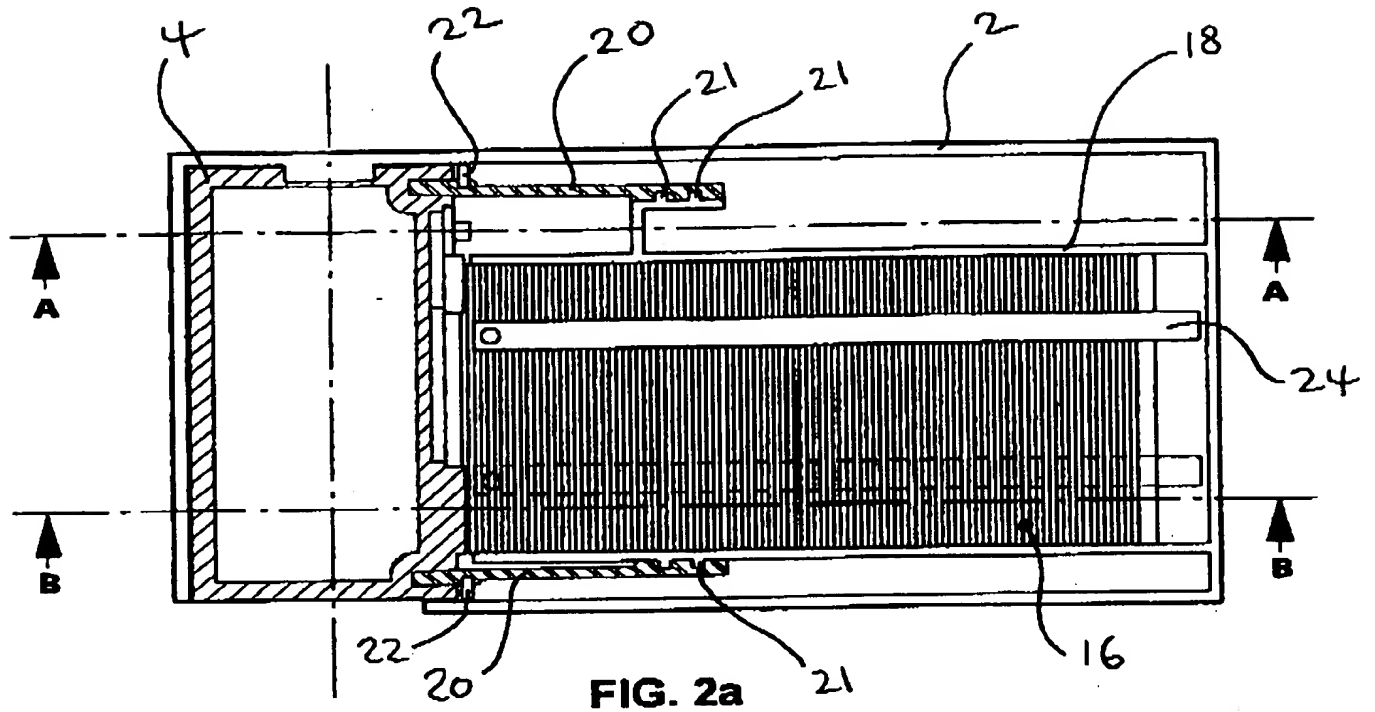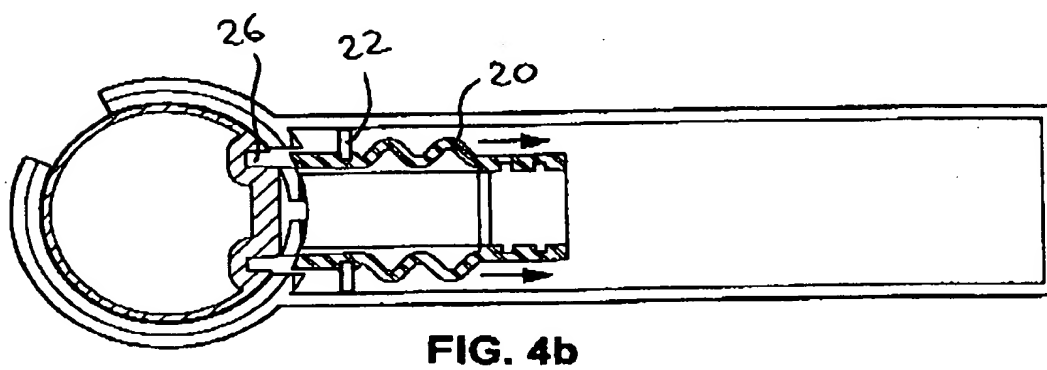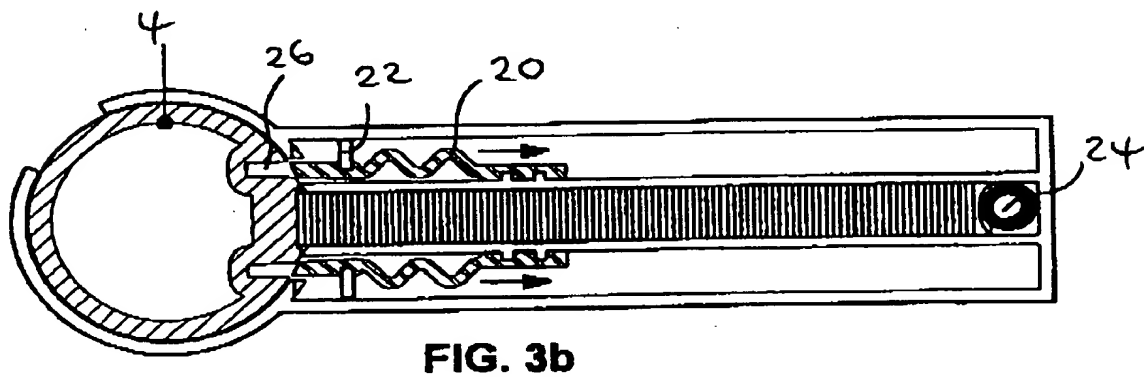

4/18

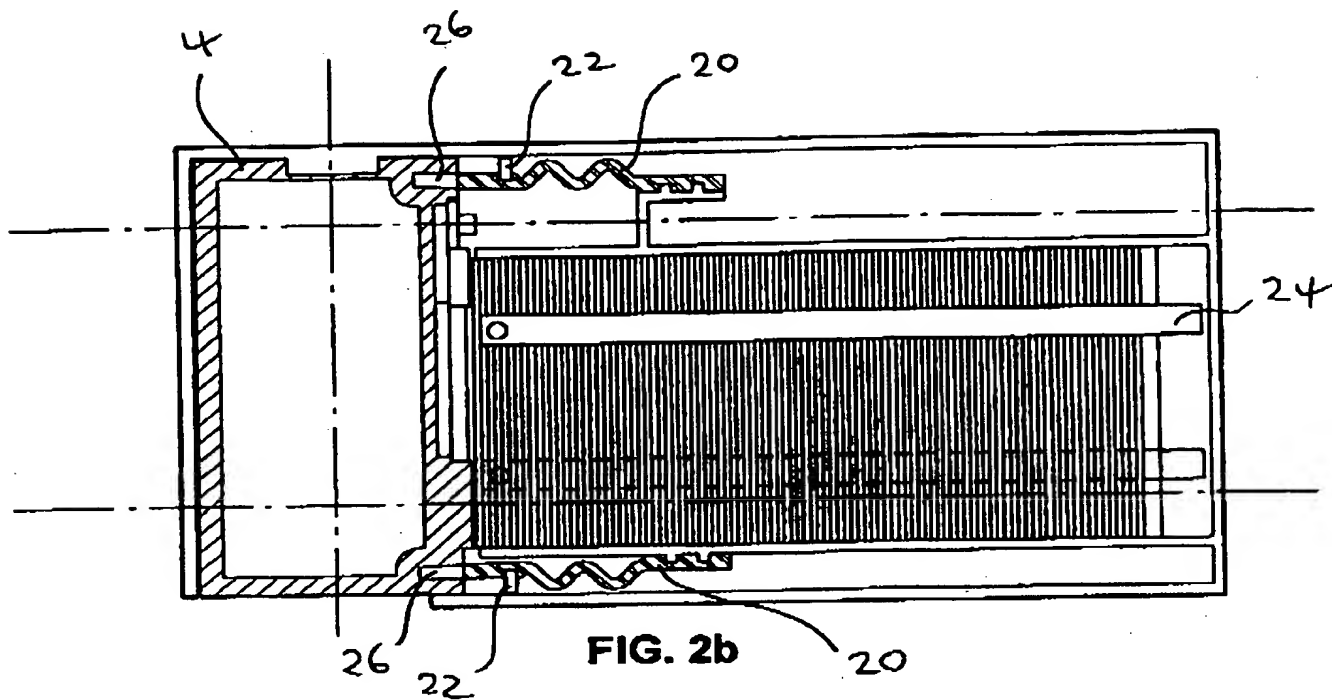

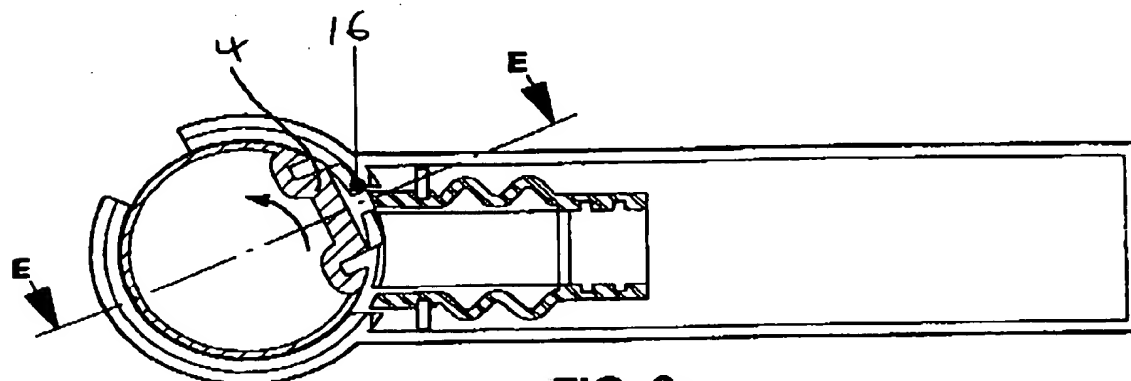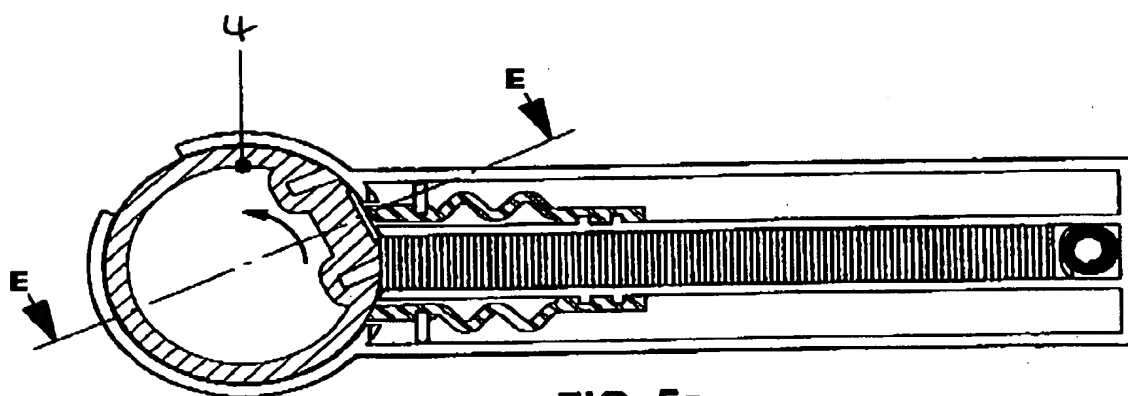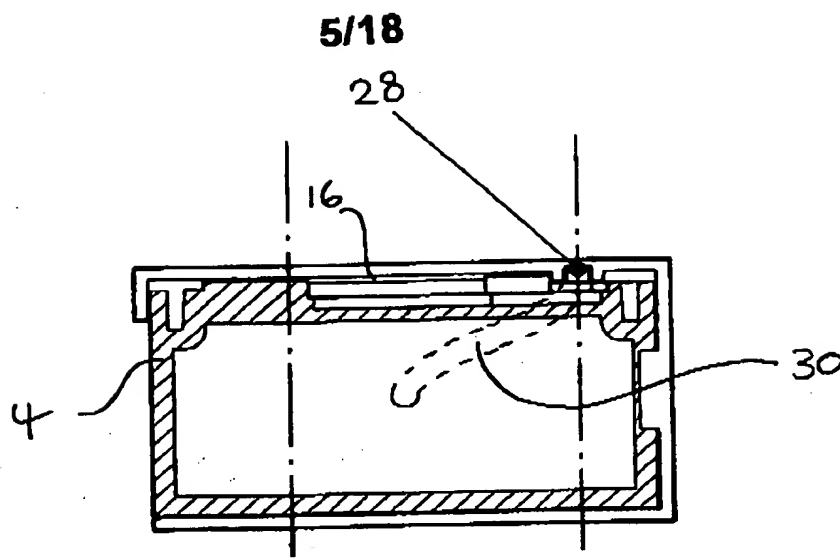



6/18

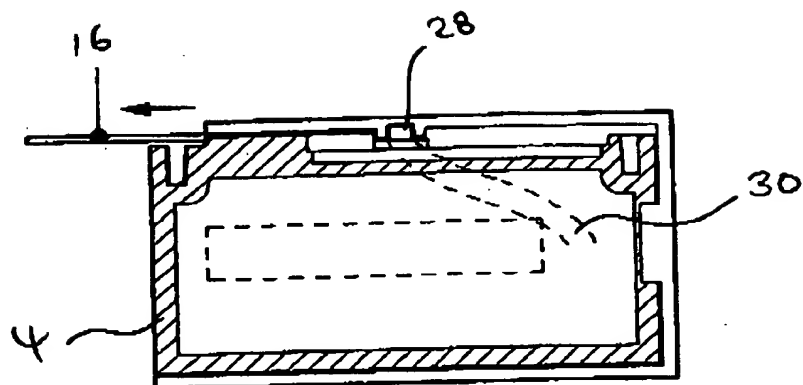


FIG. 7b

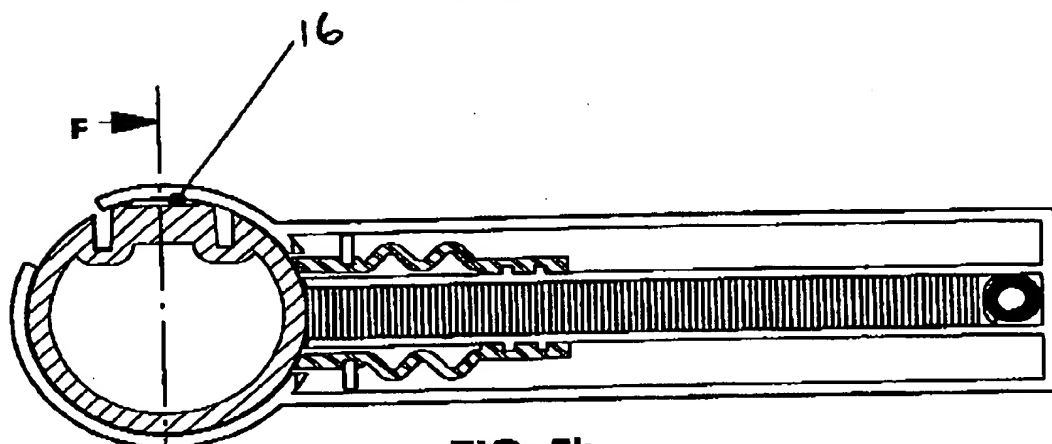


FIG. 5b

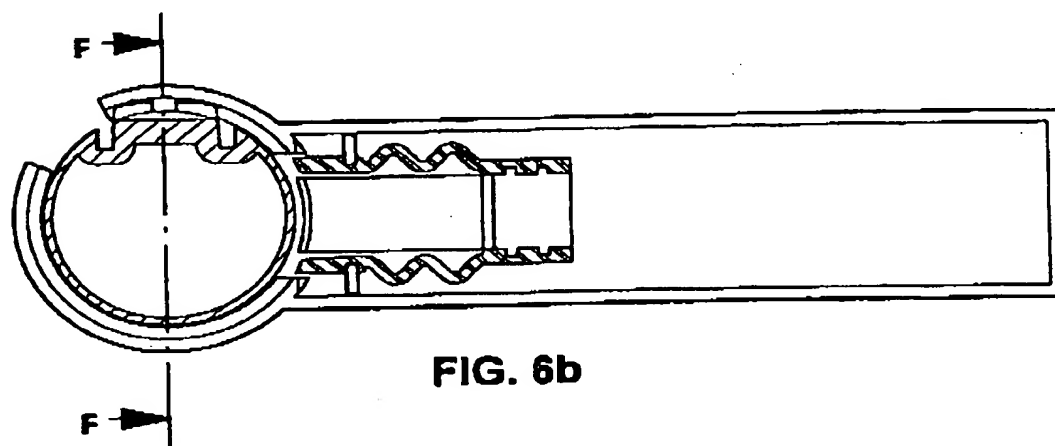


FIG. 6b

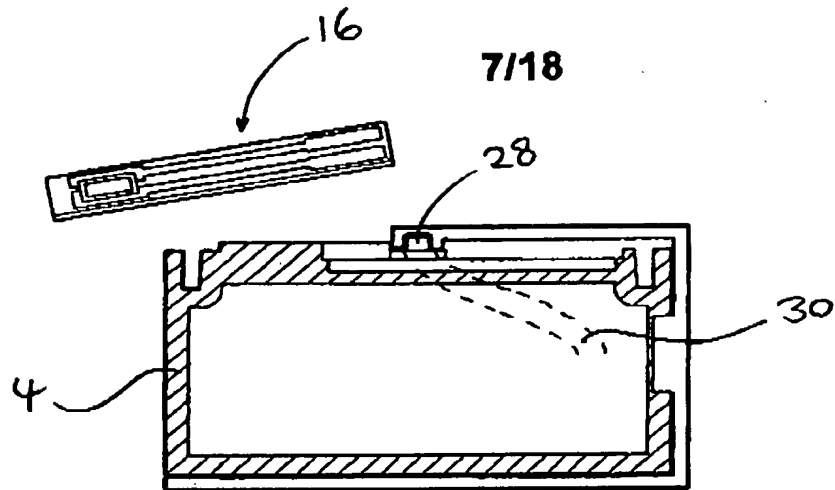


FIG. 7c

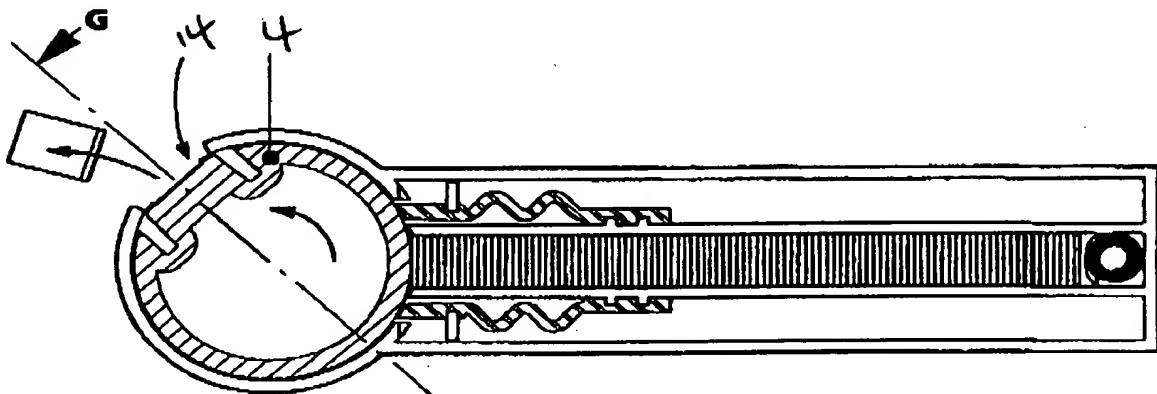


FIG. 5c

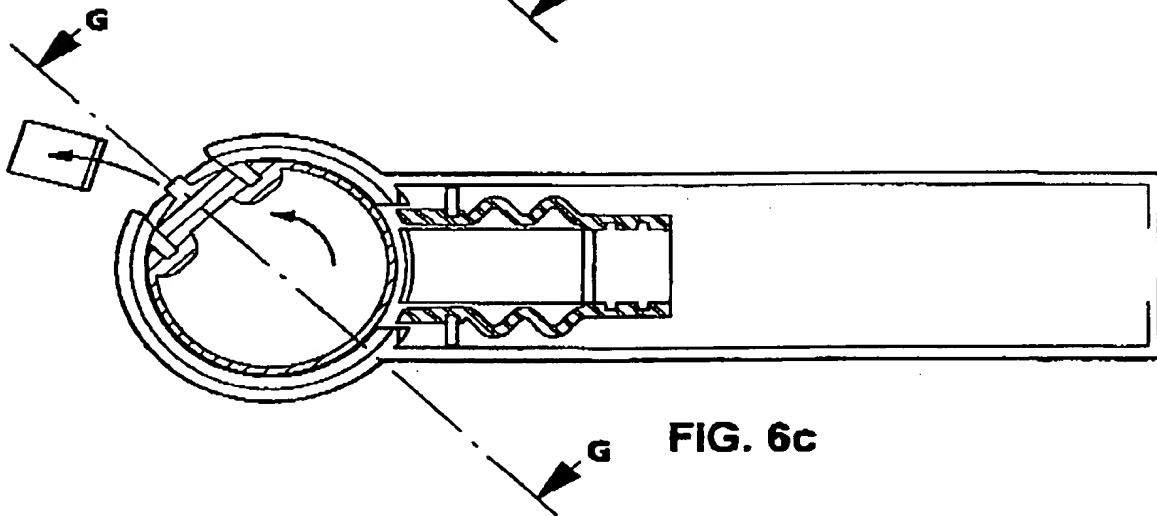


FIG. 6c

8/18

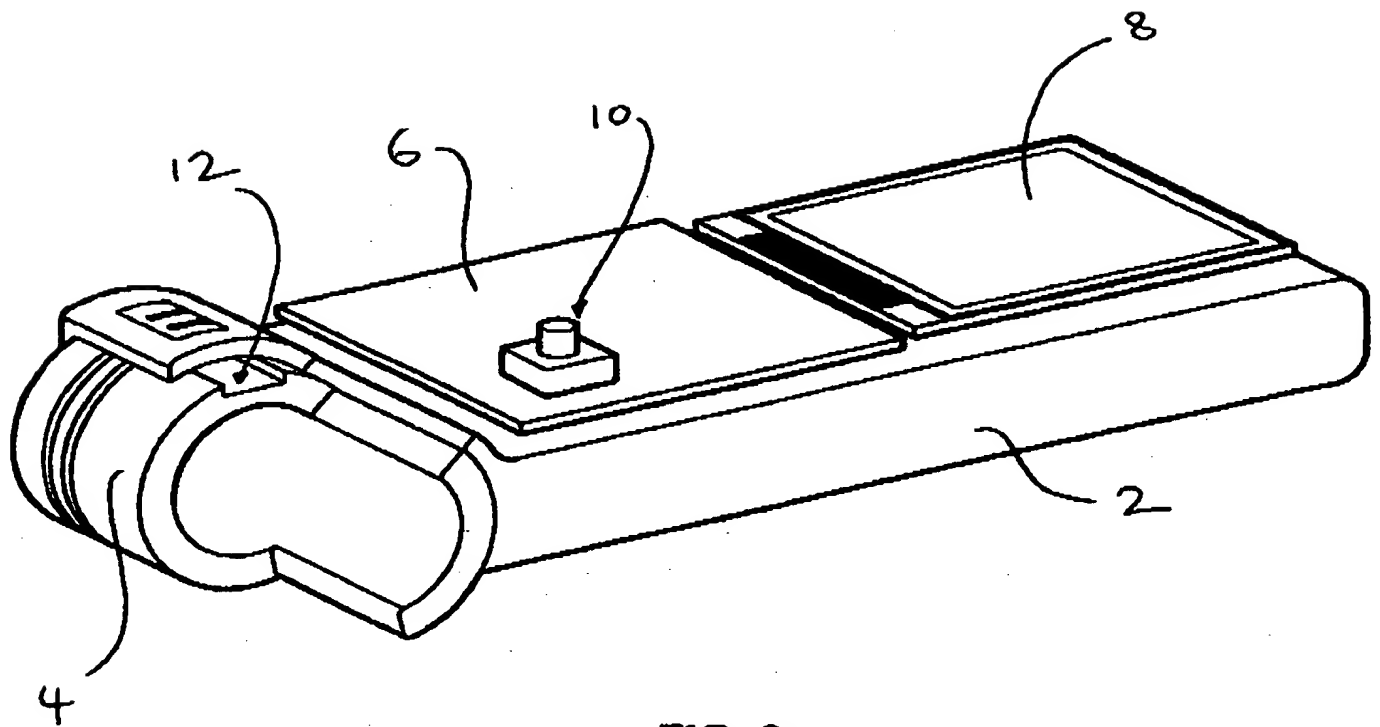


FIG. 8a

9/18








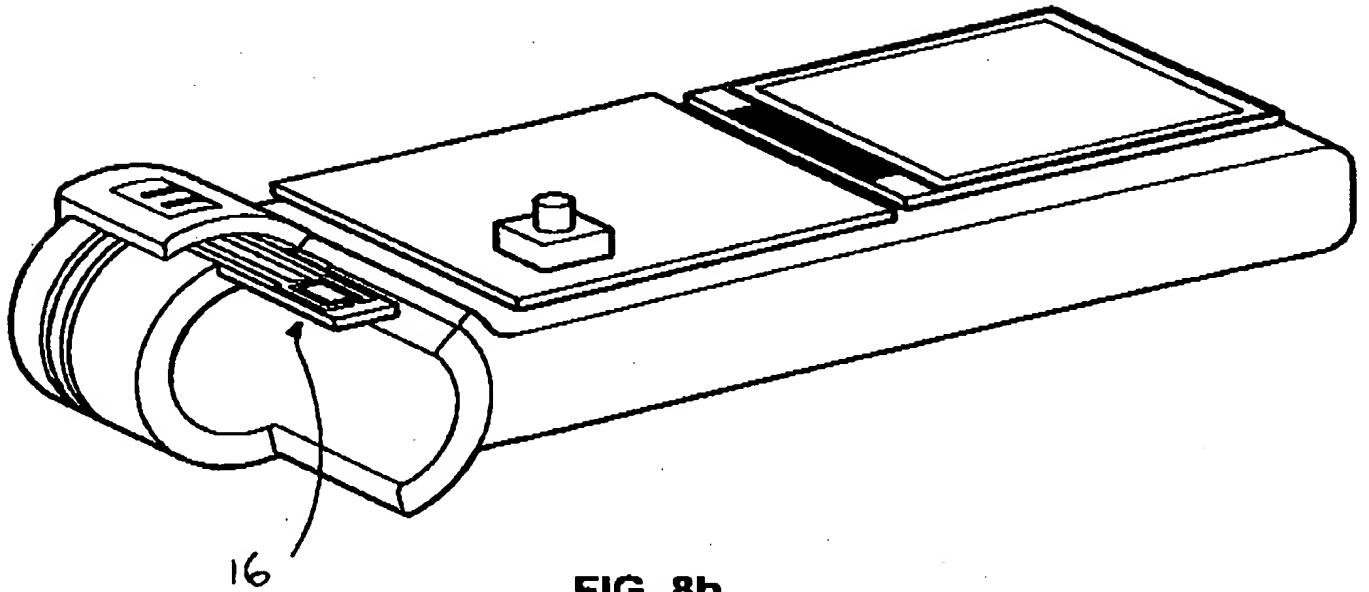


FIG. 8b





10/18

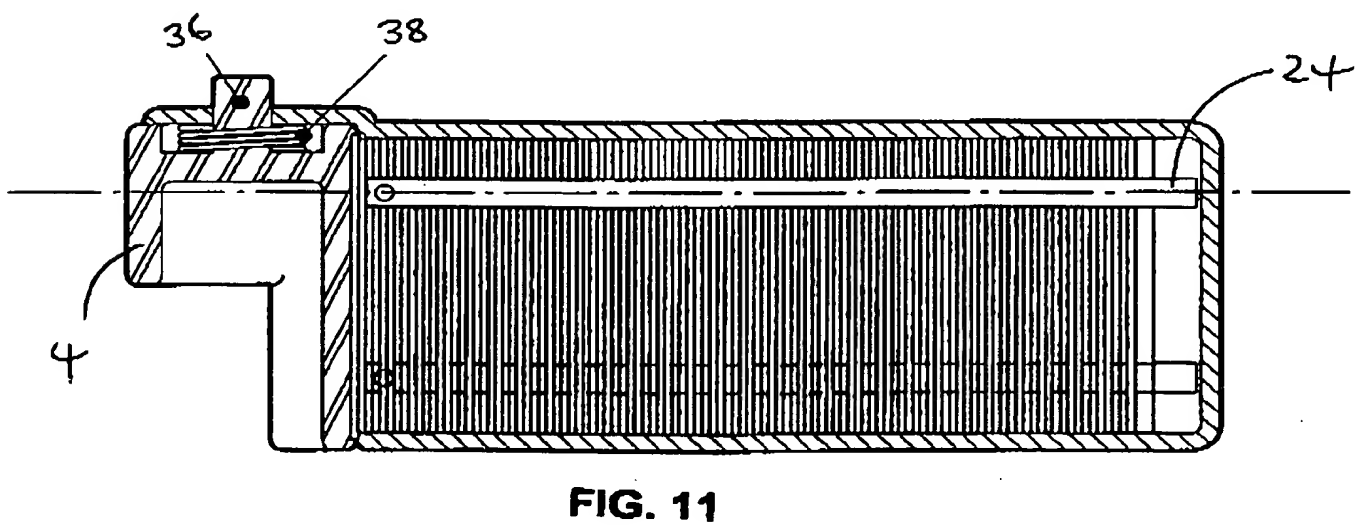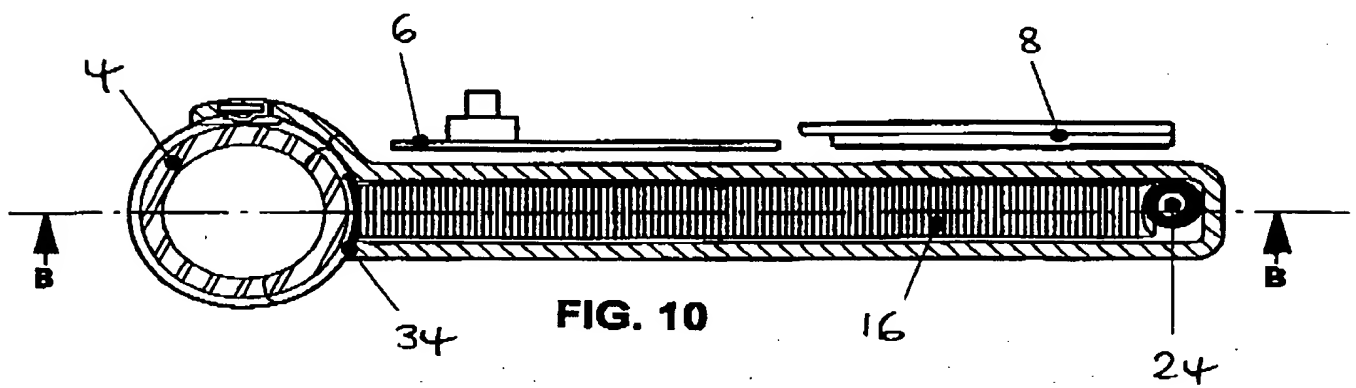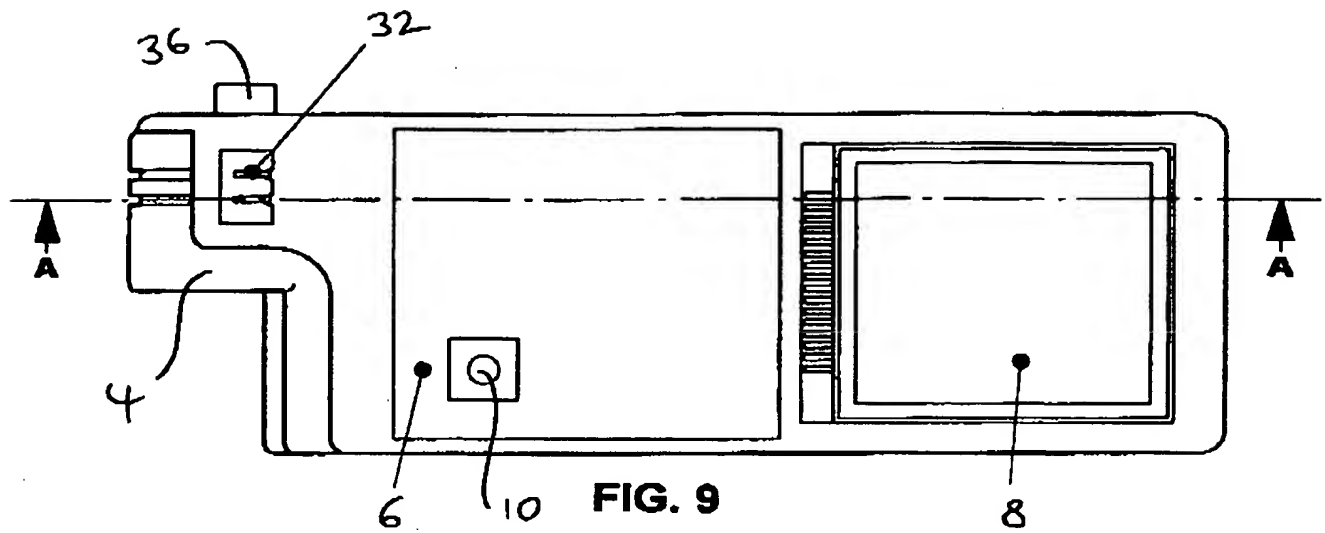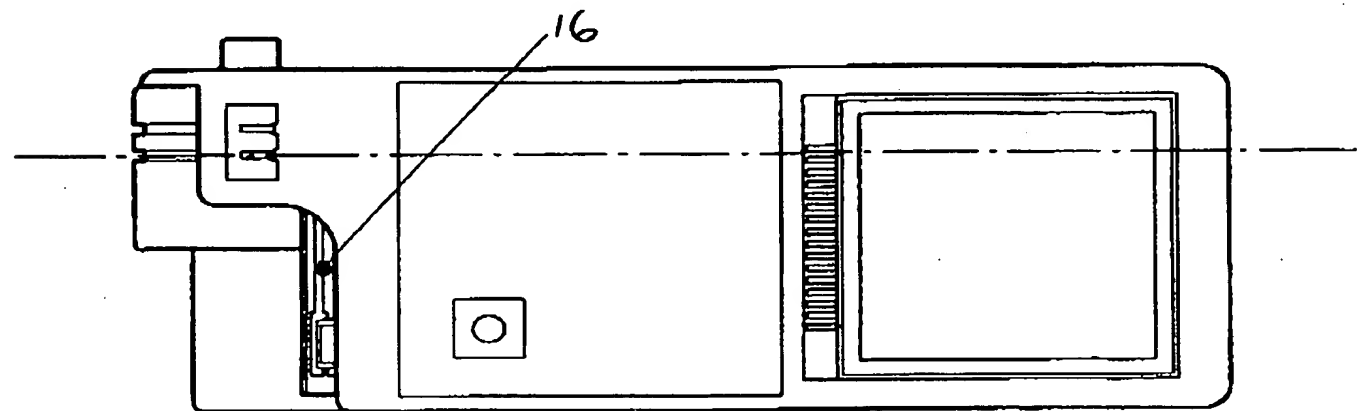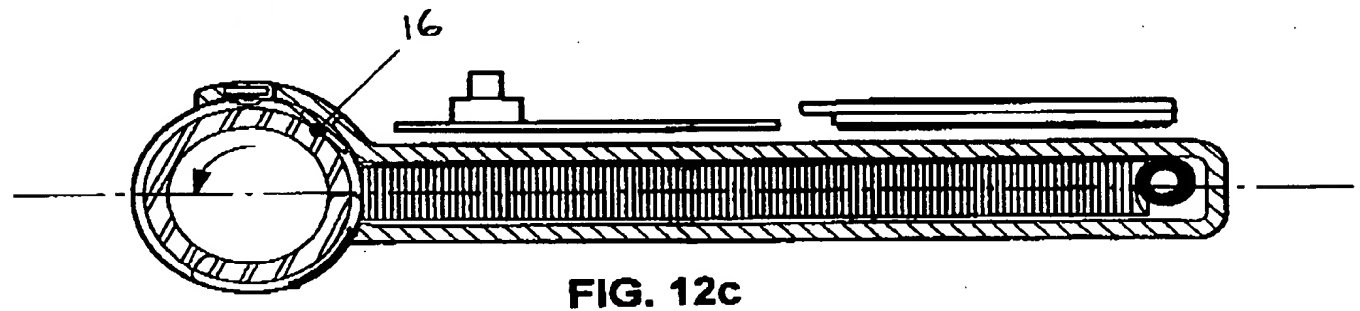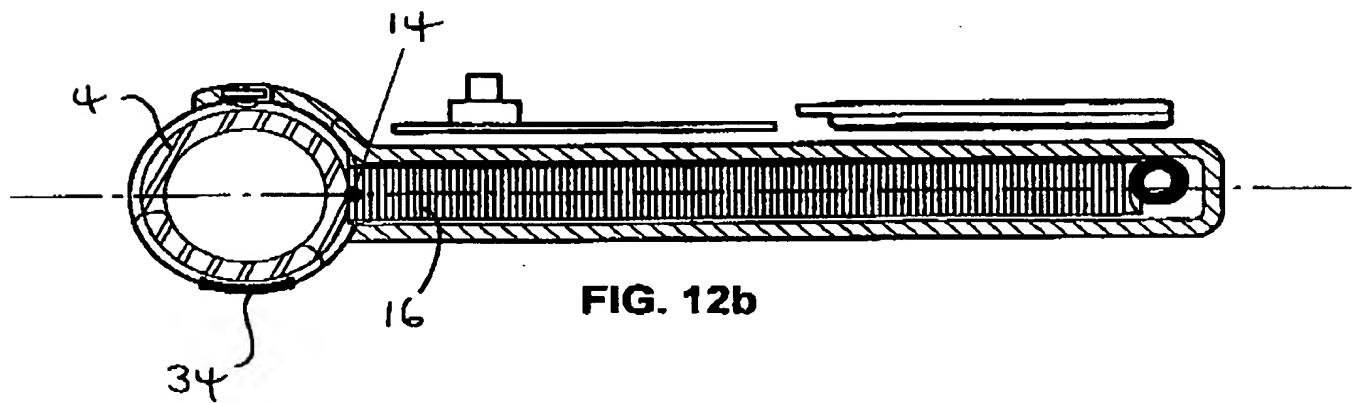

11/18

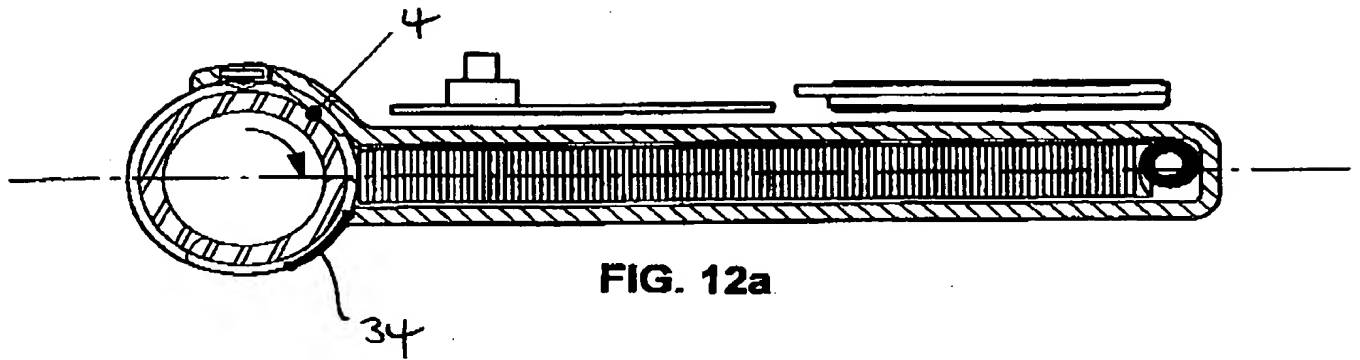

12/18

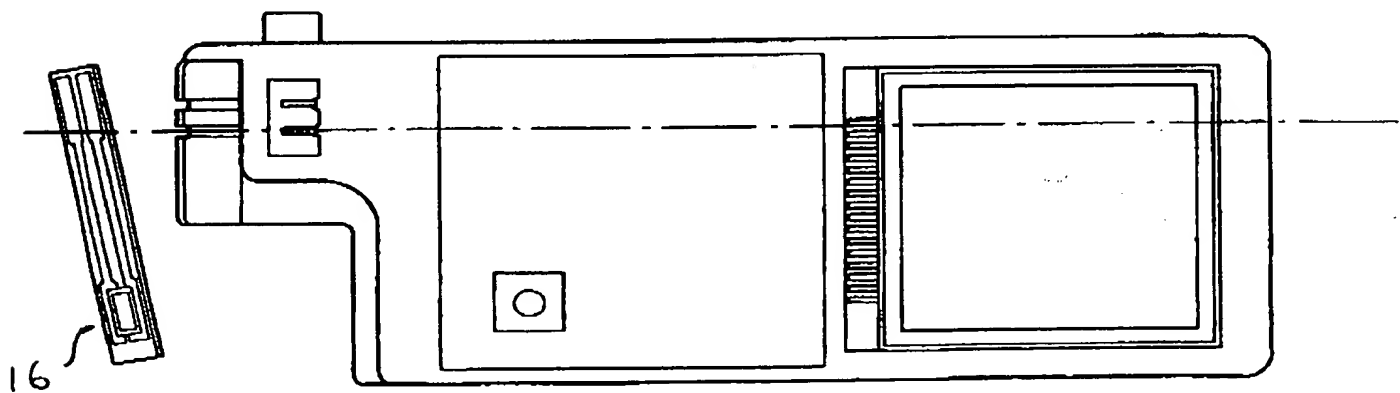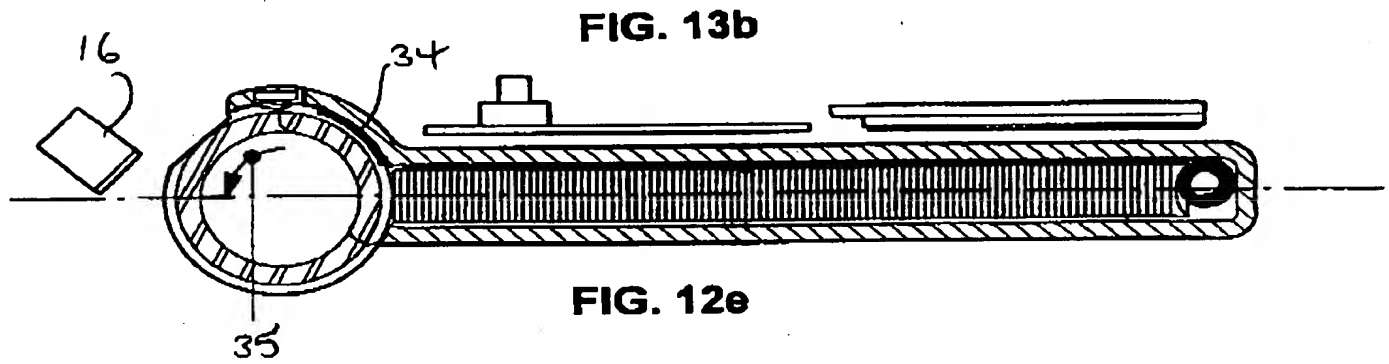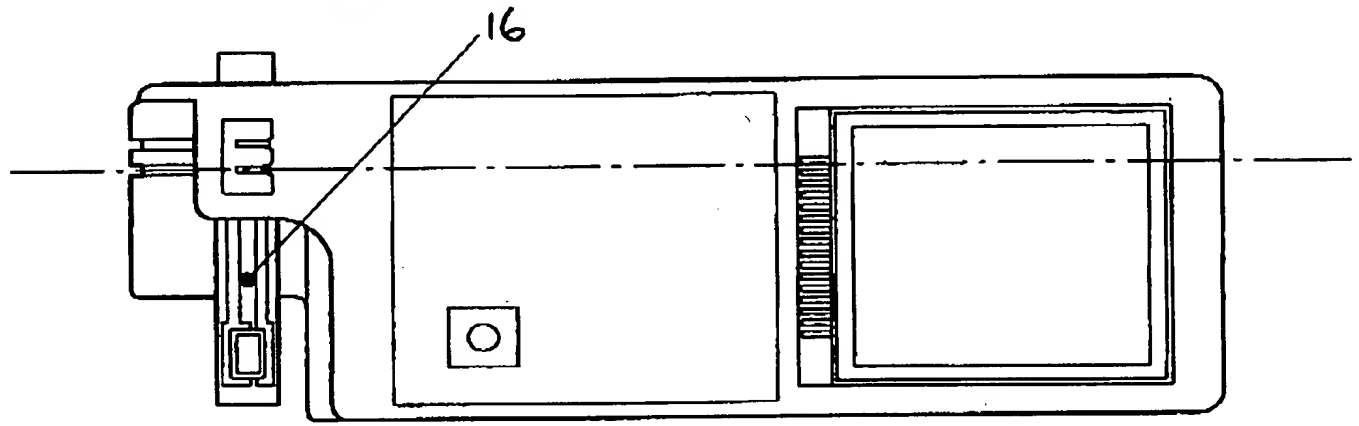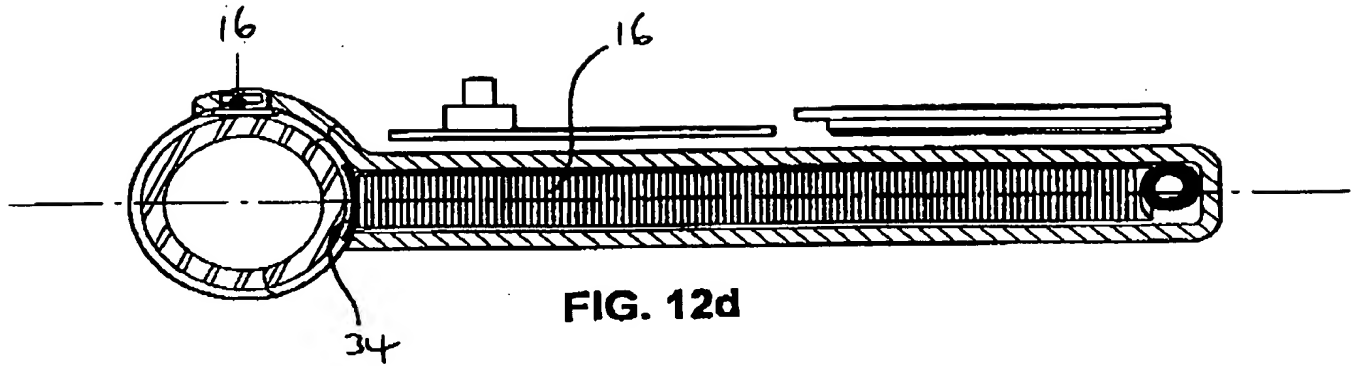

13/18

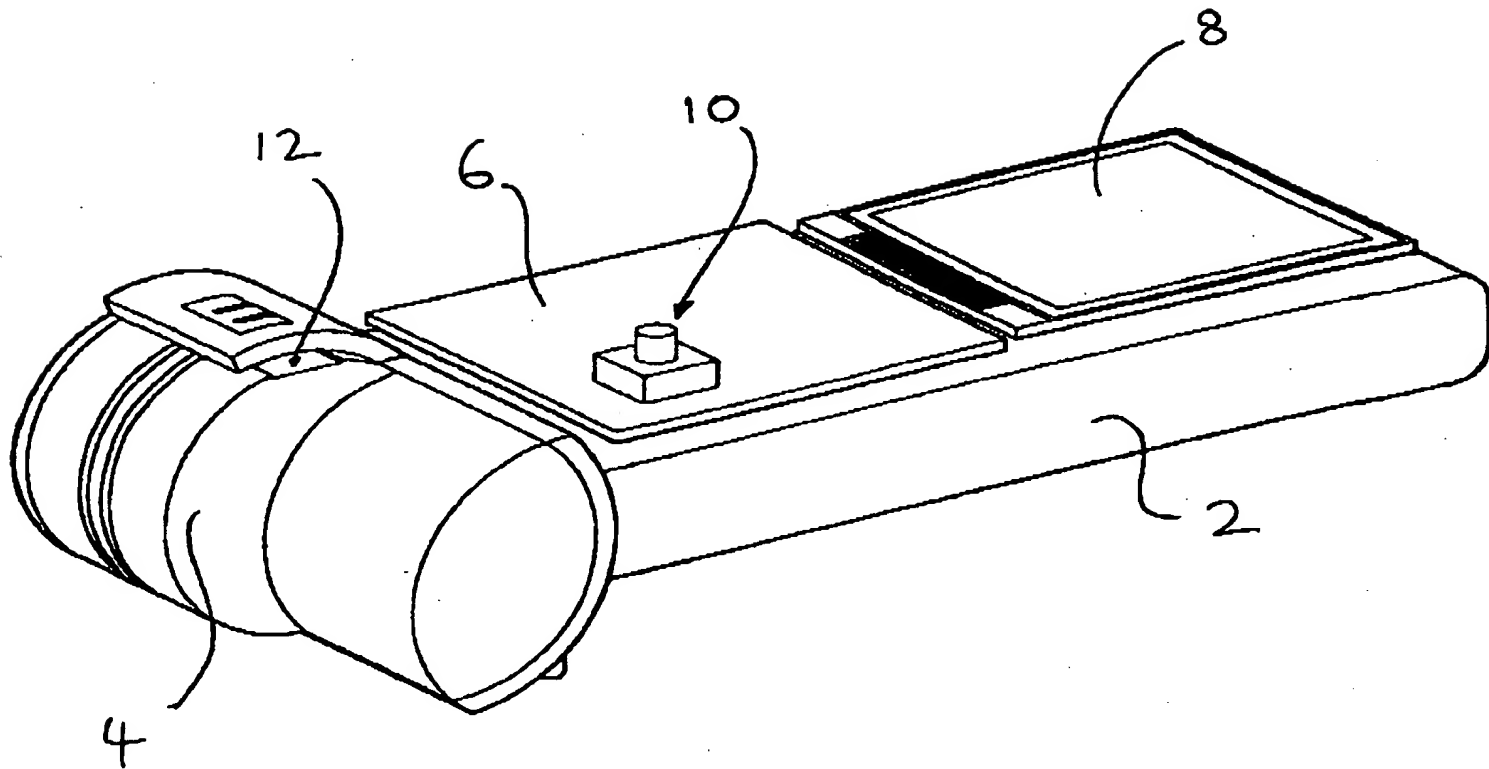


FIG. 14a



14/18












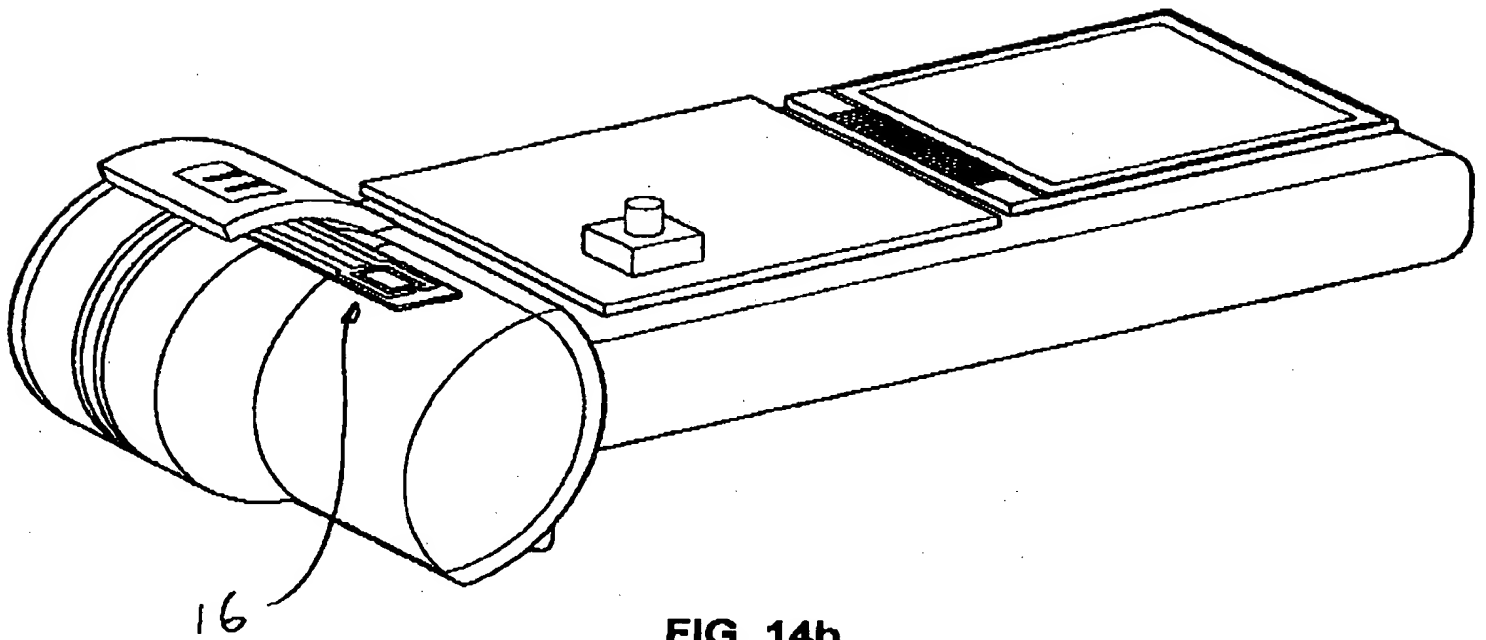


FIG. 14b

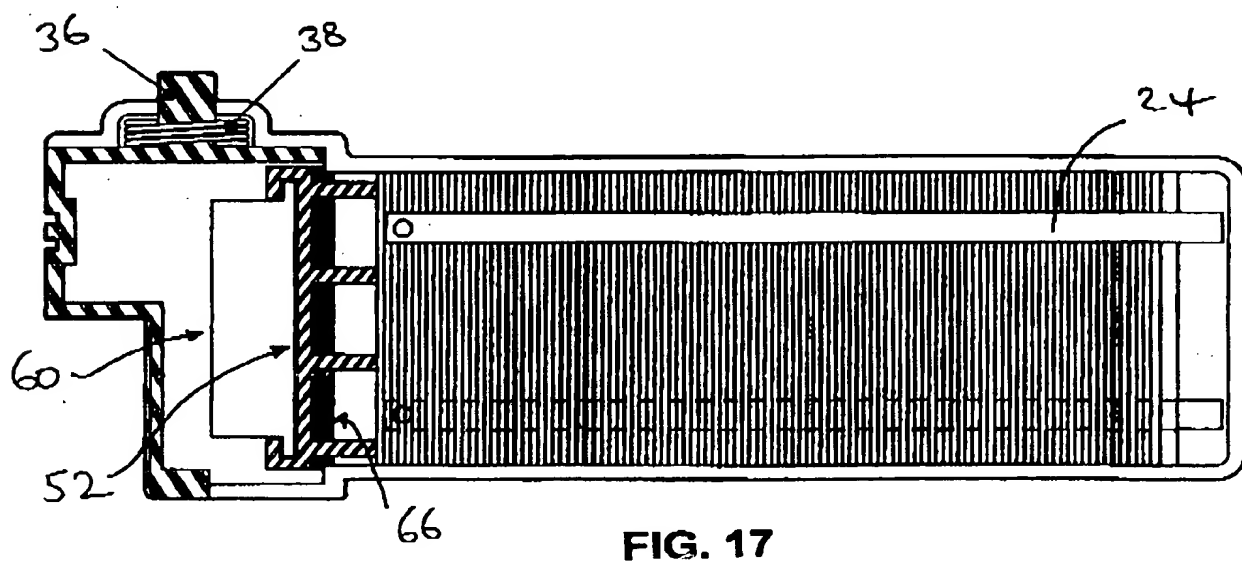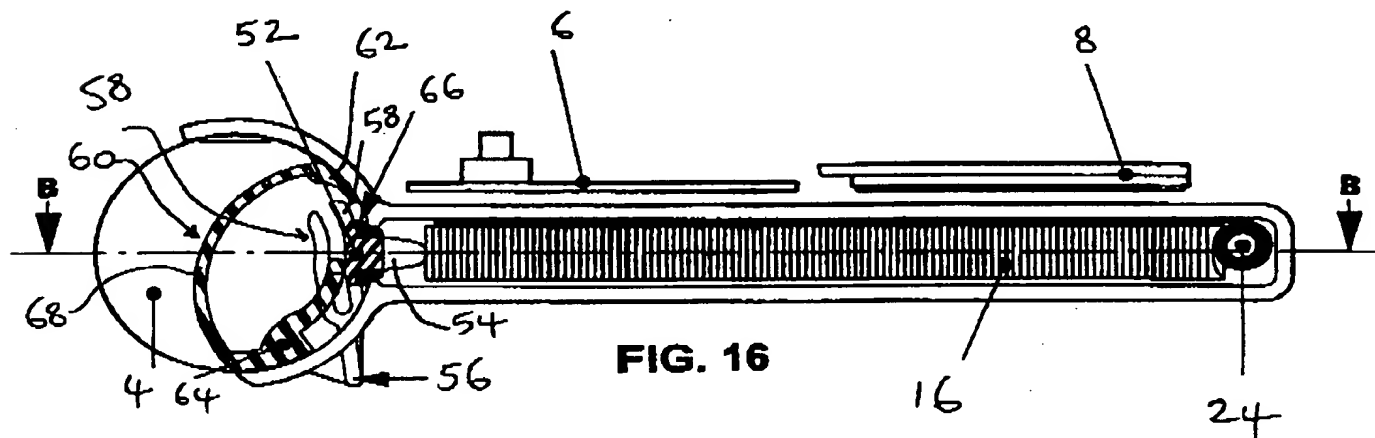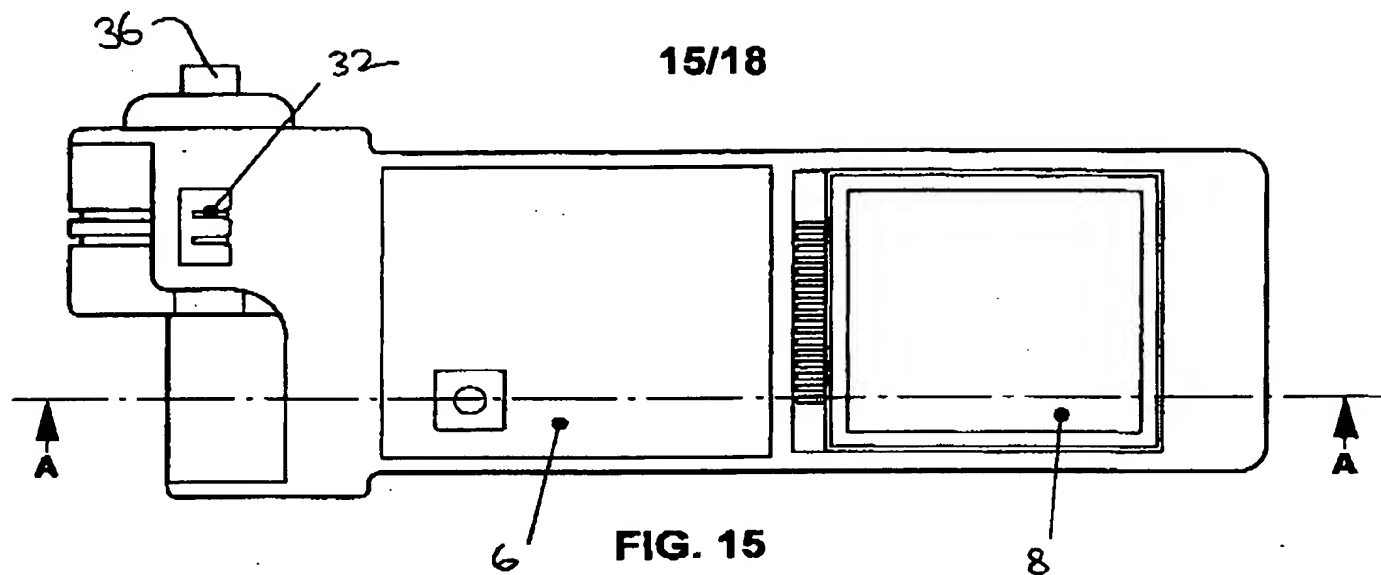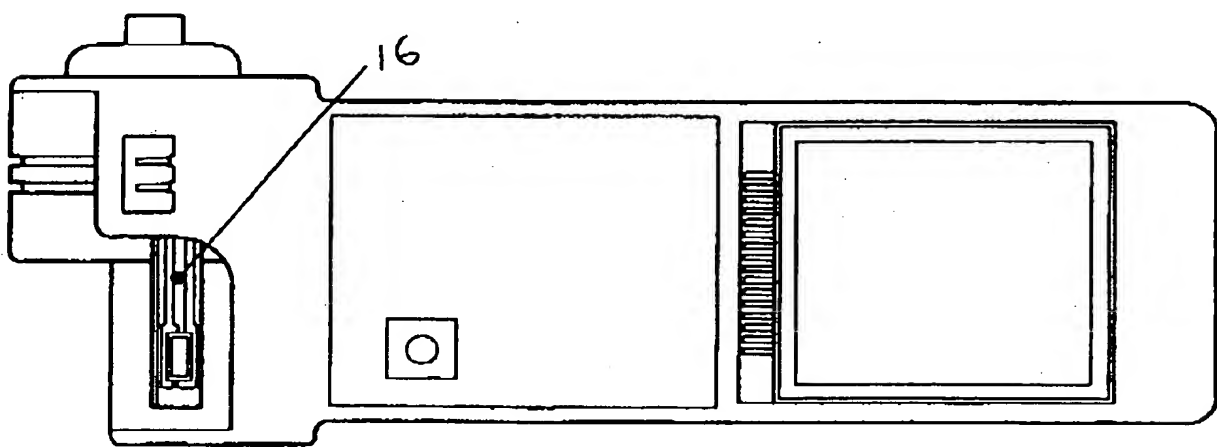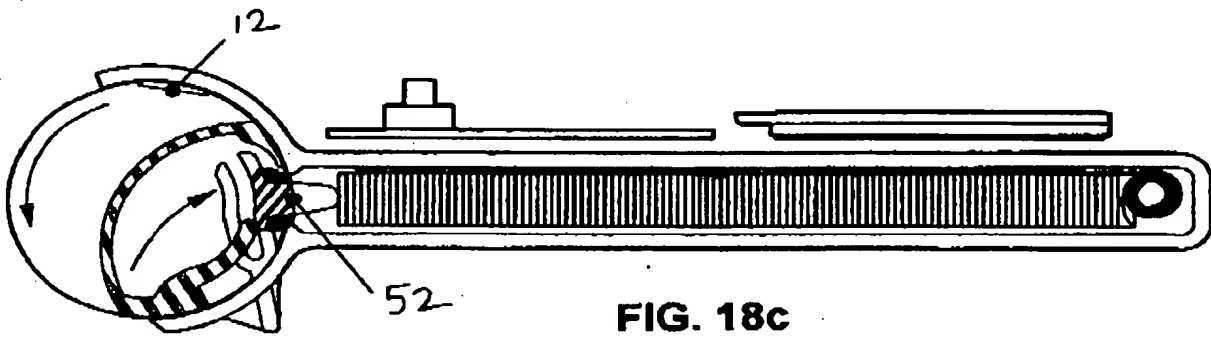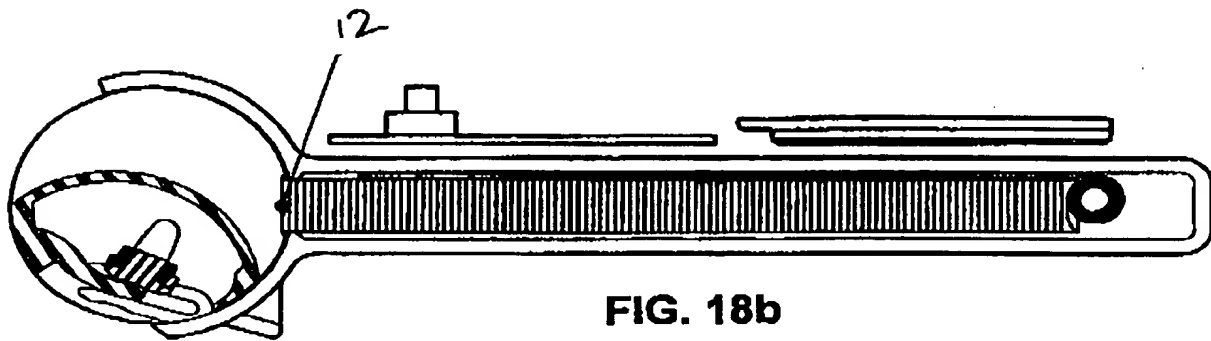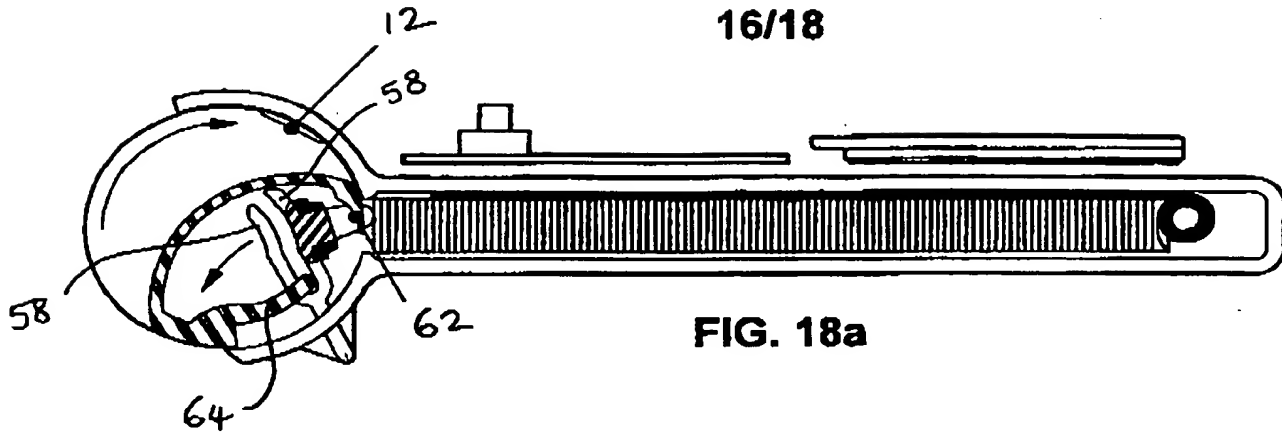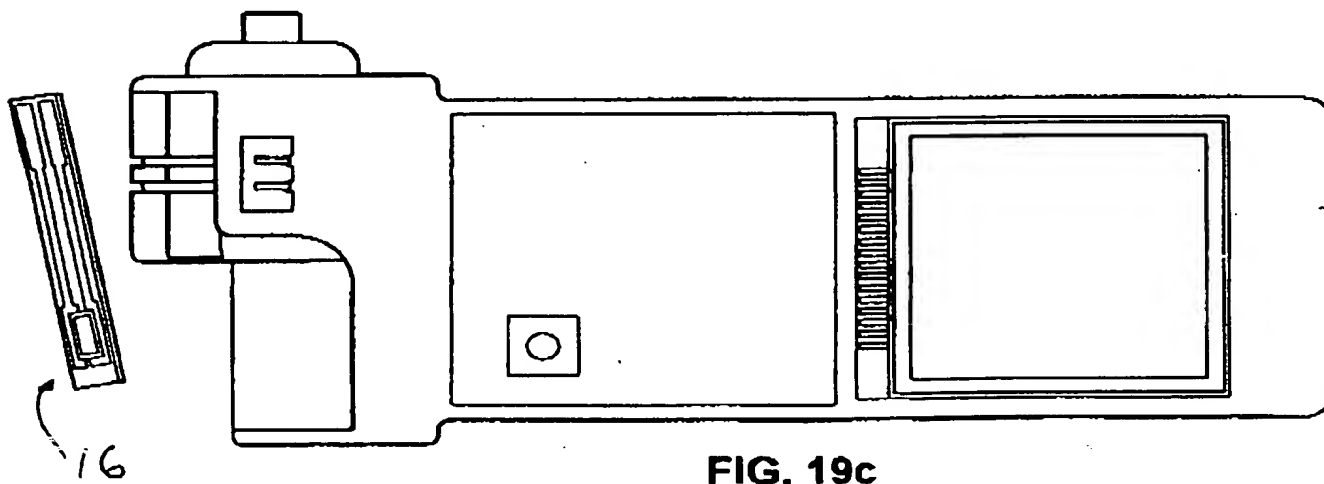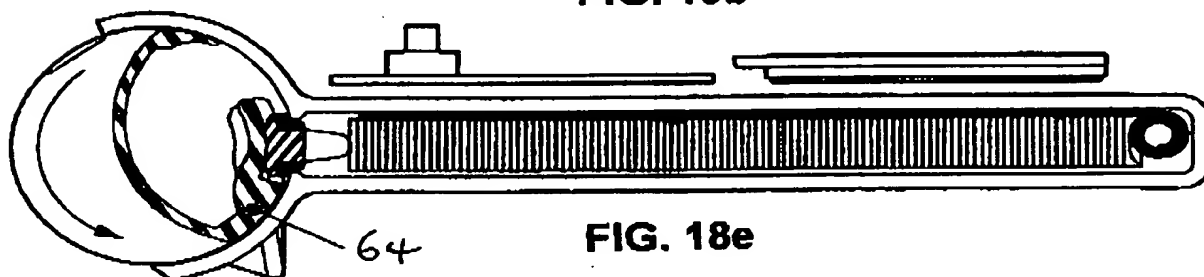

16/18

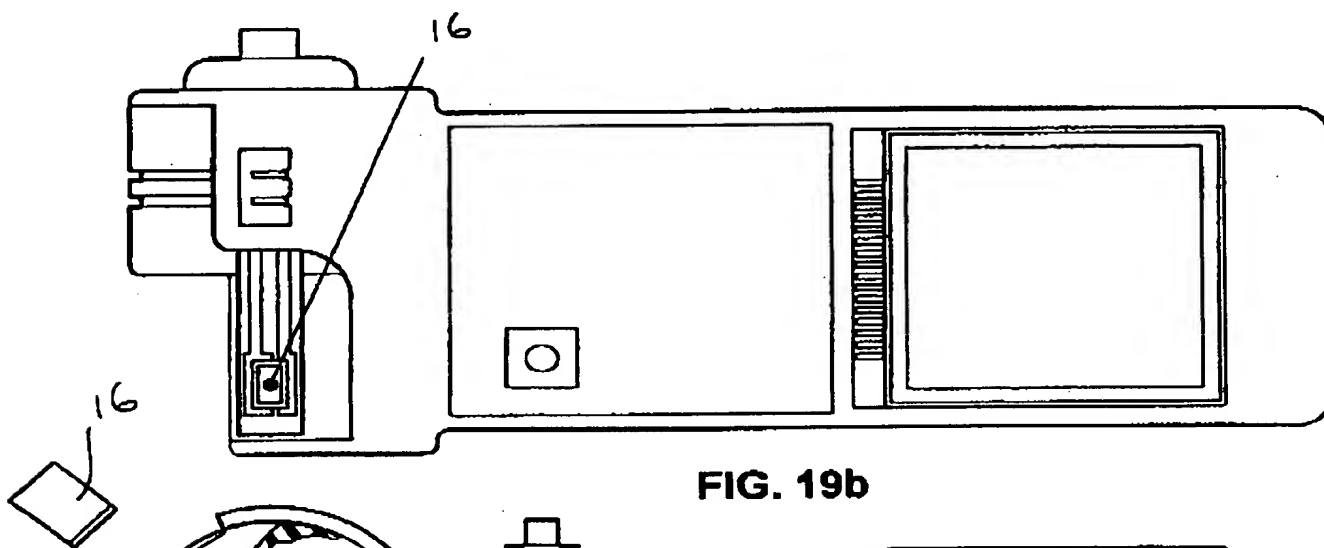

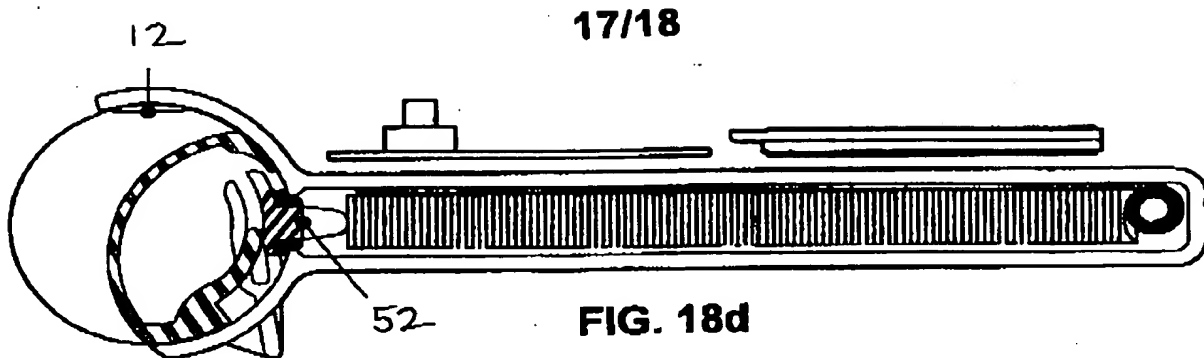

18/18

